

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
 Data File : VU062854.D
 Acq On : 17 Jan 2025 05:37
 Operator : MD/SY
 Sample : Q1072-09
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ91

Quant Time: Jan 17 06:19:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 16 23:11:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	88161	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	85197	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	39638	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	20905	4.281	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.904	69	18292	4.657	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.557	65	11229	4.439	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.800%
20) 2-Butanone-d5	4.605	46	52356	52.465	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.920%
24) Chloroform-d	5.049	84	57939	4.823	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.689	65	34439	5.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
32) Benzene-d6	5.714	84	96222	4.620	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.679	67	28758	4.980	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.888	98	89285	4.400	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	8.171	79	13236	4.599	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.000%
46) 2-Hexanone-d5	8.621	63	38736	42.790	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.580%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	24133	4.990	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	12.183	152	34124	5.175	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.400%
Target Compounds					Qvalue	
17) Methyl tert-butyl Ether	3.351	73	1996	0.133	ug/L	# 85
19) 1,1-Dichloroethane	3.865	63	2162	0.206	ug/L	99
34) Trichloroethene	6.531	95	3935	0.471	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
Data File : VU062854.D
Acq On : 17 Jan 2025 05:37
Operator : MD/SY
Sample : Q1072-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCQ91

Quant Time: Jan 17 06:19:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 16 23:11:57 2025
Response via : Initial Calibration




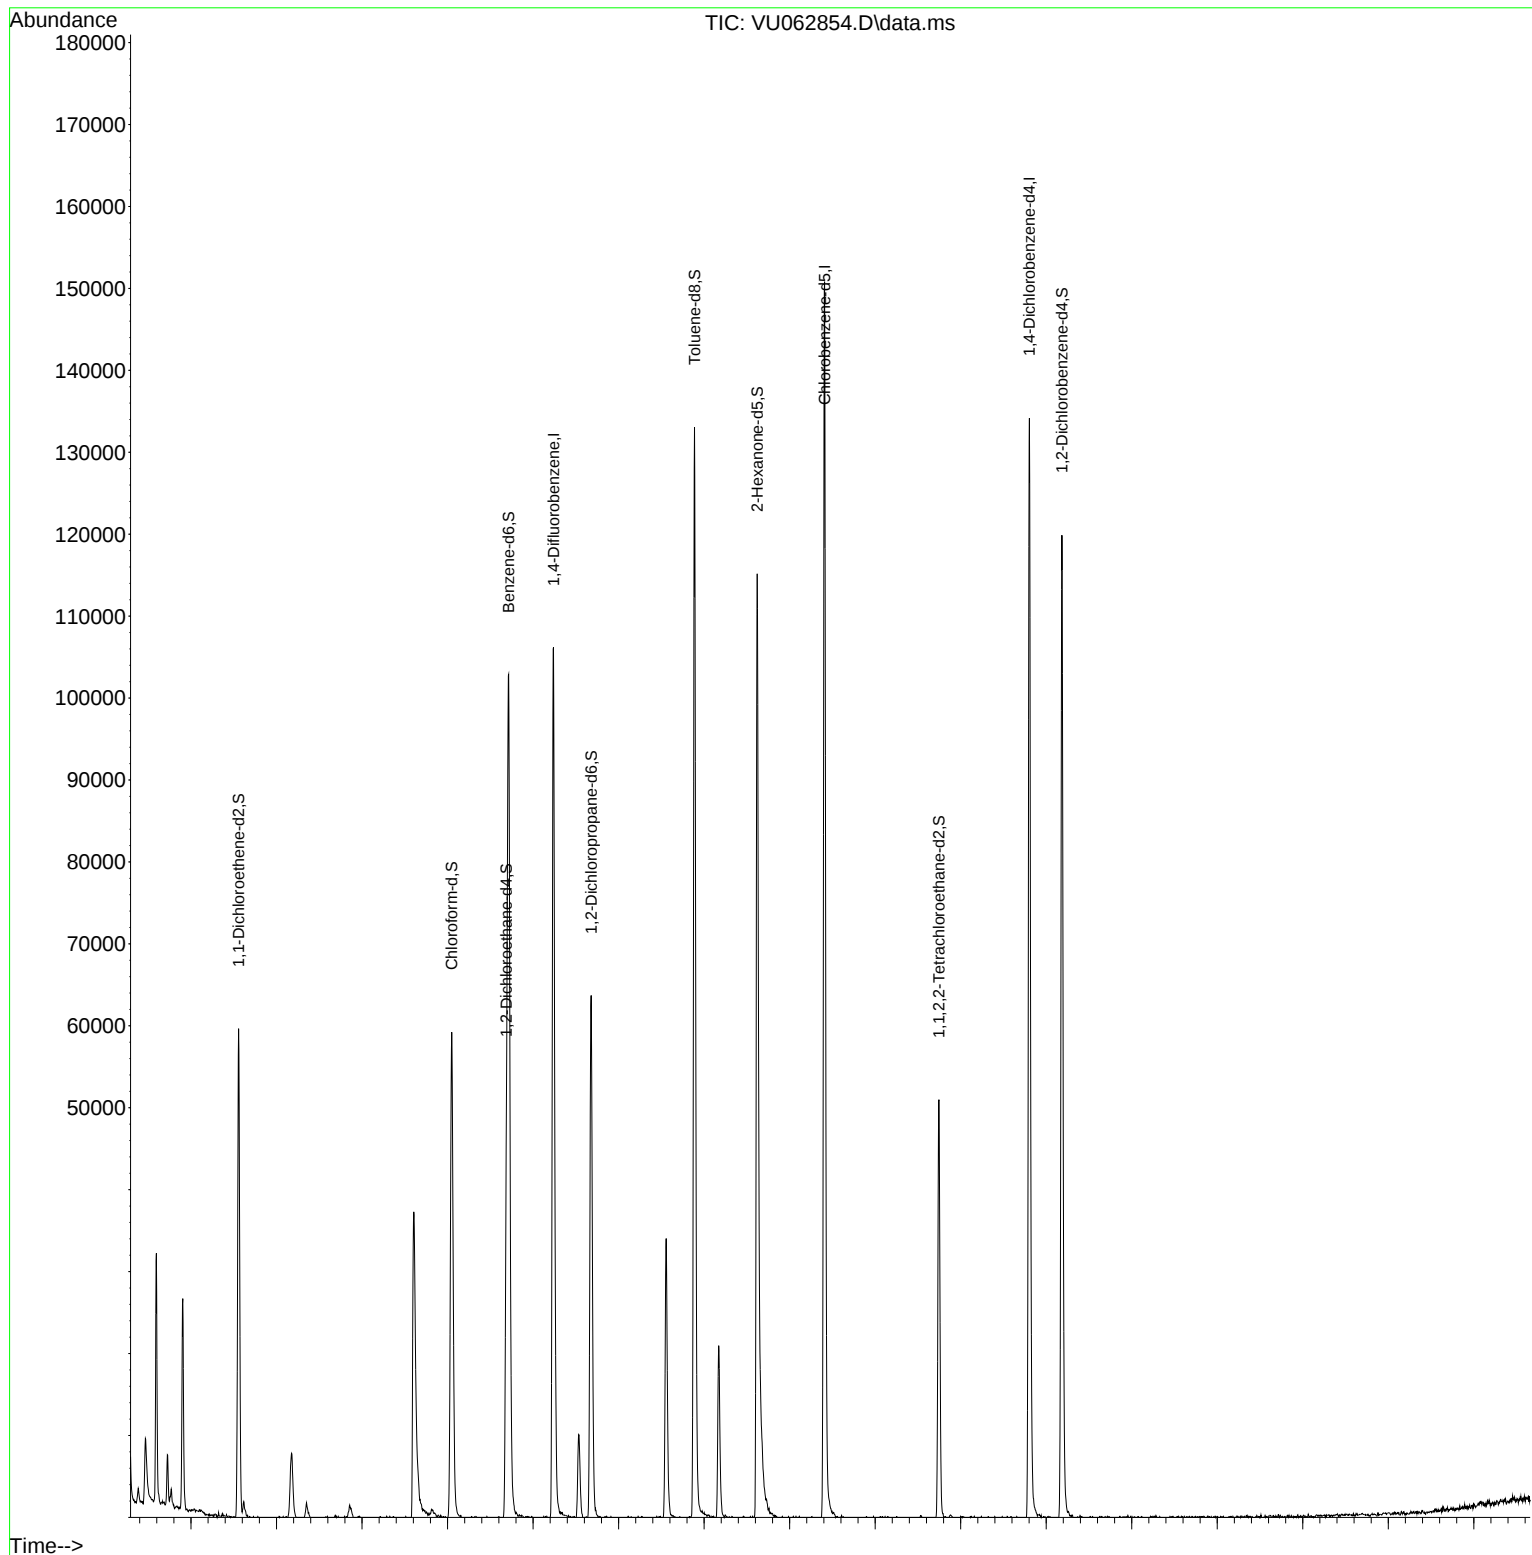


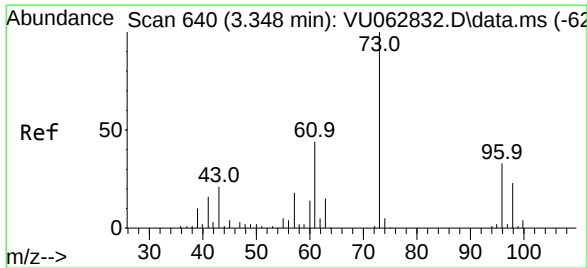

#17
Methyl tert-butyl Ether
Concen: 0.133 ug/L
RT: 3.351 min Scan# 641
Delta R.T. 0.003 min
Lab File: VU062854.D
Acq: 17 Jan 2025 05:37




Instrument :
MSVOA_U
ClientSampleId :
GCQ91


Tgt Ion: 73	Resp: 1996
Ion Ratio	Lower Upper
73 100	
43 16.0	16.2 24.4#
57 8.6	14.6 22.0#

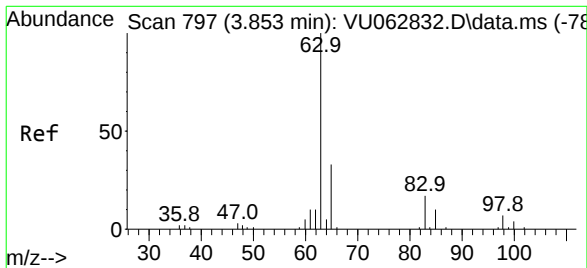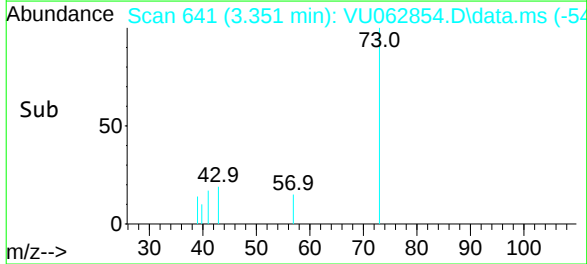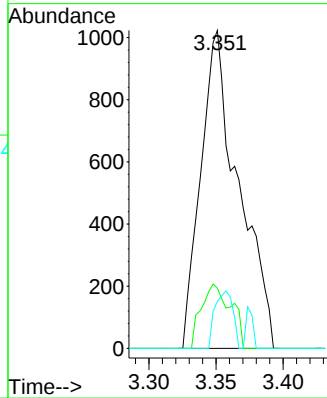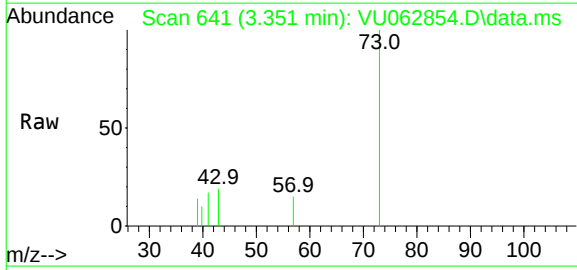

#19
1,1-Dichloroethane
Concen: 0.206 ug/L
RT: 3.865 min Scan# 801
Delta R.T. 0.013 min
Lab File: VU062854.D
Acq: 17 Jan 2025 05:37


Tgt Ion: 63	Resp: 2162
Ion Ratio	Lower Upper
63 100	
65 29.3	20.7 38.5
83 15.9	10.5 19.5

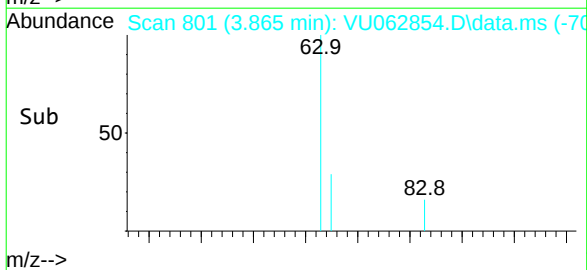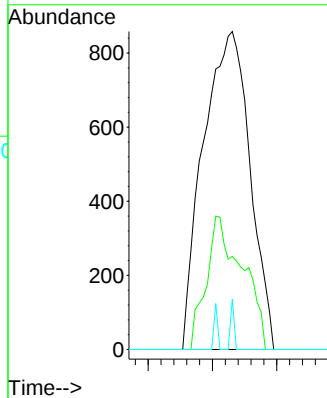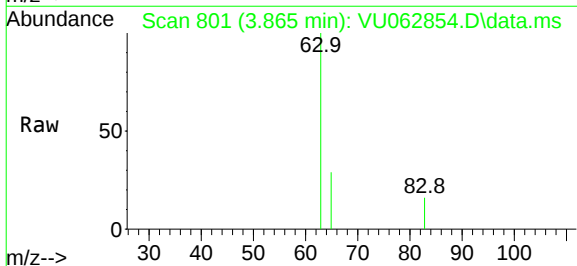

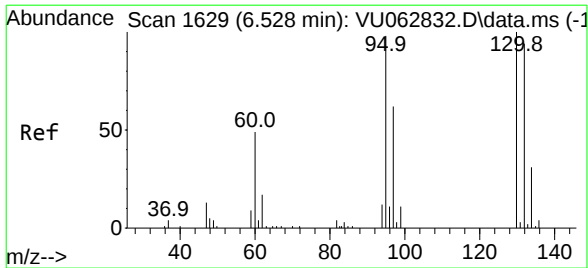

#34
 Trichloroethene
 Concen: 0.471 ug/L
 RT: 6.531 min Scan# 16
 Delta R.T. 0.003 min
 Lab File: VU062854.D
 Acq: 17 Jan 2025 05:37

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ91

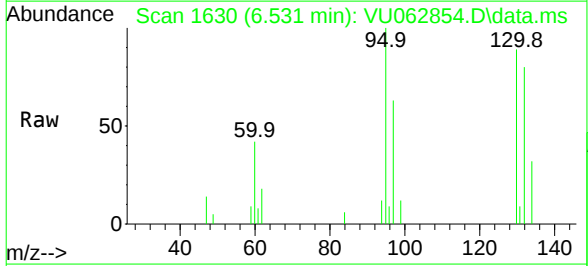

Tgt Ion:	95	Resp:	3935
Ion	Ratio	Lower	Upper
95	100		
97	63.2	47.5	88.3
132	79.7	66.9	124.3
130	89.4	68.6	127.4

