
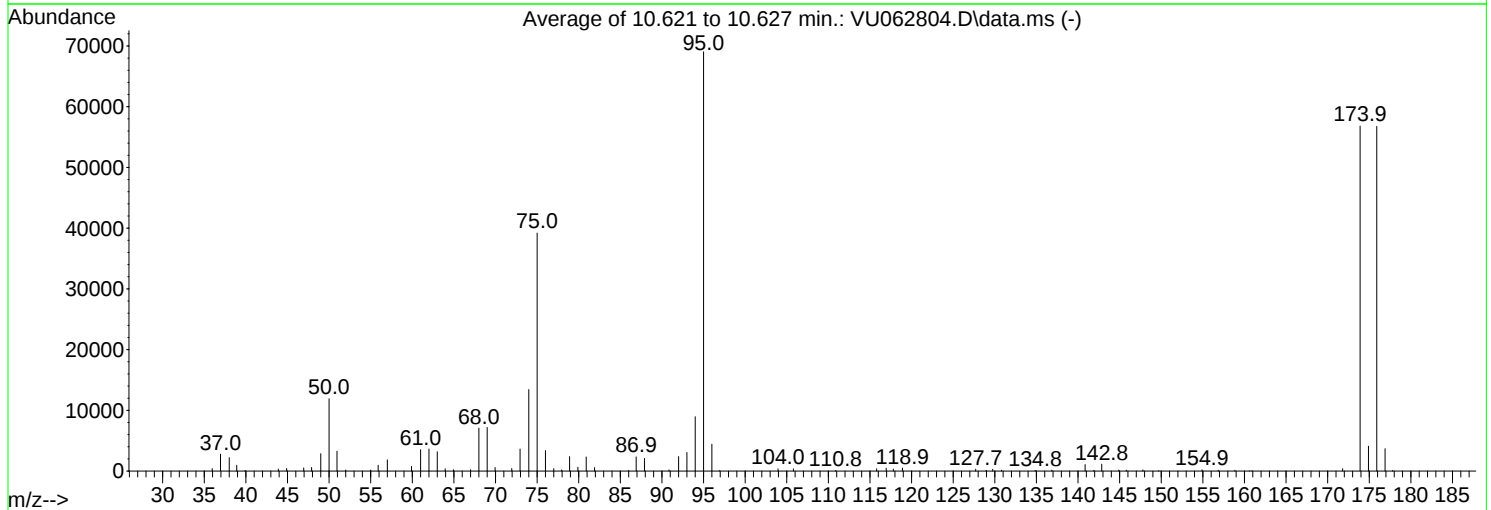


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
Data File : VU062804.D
Acq On : 16 Jan 2025 08:38
Operator : MD/SY
Sample : BFB062
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB062

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 16 23:11:57 2025

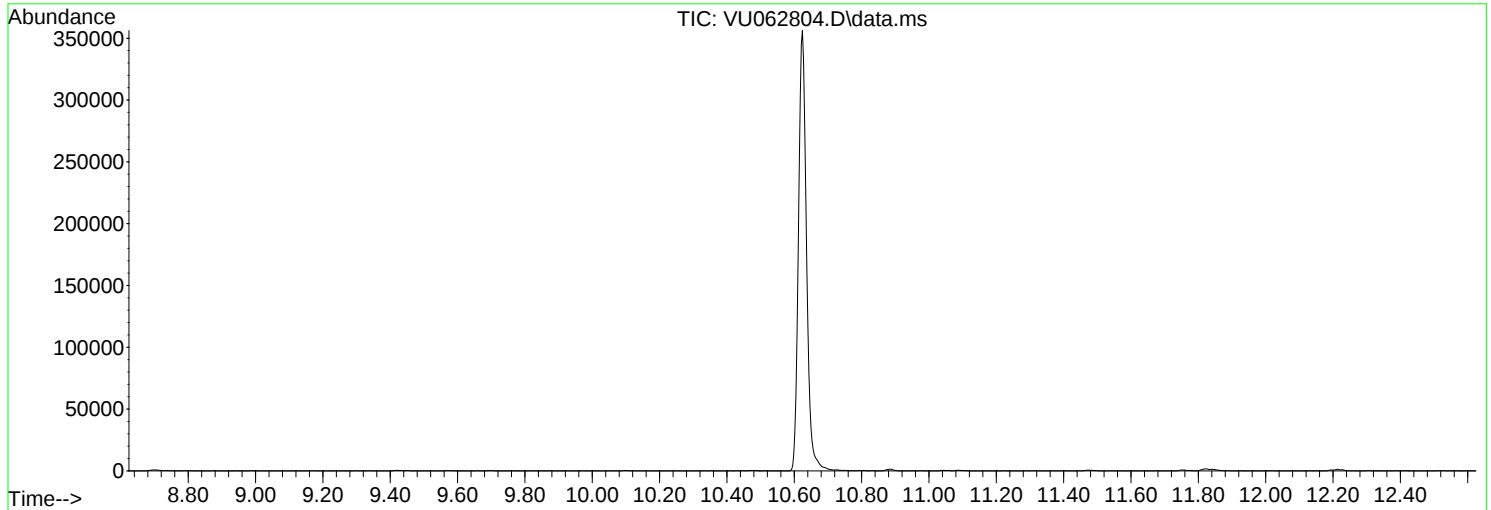

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	11911	PASS
75	95	30	80	56.8	39200	PASS
95	95	100	100	100.0	69053	PASS
96	95	5	9	6.4	4425	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.3	56819	PASS
175	174	5	9	7.2	4093	PASS
176	174	95	101	99.9	56757	PASS
177	176	5	9	6.5	3685	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB062

m/z	Abundance
36.00	397.0
37.00	2717.0
38.00	2249.0
38.90	1002.0
39.90	161.0
44.00	334.0
44.90	383.0
47.00	493.0
47.90	531.0
49.00	2810.0
50.00	12125.0
50.90	3452.0
52.00	175.0
55.00	180.0
55.90	1043.0
57.00	1904.0
59.90	761.0
61.00	3702.0
62.00	3728.0
63.00	3252.0
63.90	369.0
64.90	220.0
67.00	227.0
68.00	7087.0
69.00	6925.0
69.90	588.0
71.90	429.0
73.00	3567.0
74.00	13679.0
75.00	39480.0
76.00	3461.0
77.00	417.0
77.90	250.0
78.90	2412.0
80.00	708.0
80.90	2395.0
81.90	562.0
86.90	2456.0
87.90	2162.0
90.80	213.0
92.00	2359.0
93.00	3214.0
94.00	8816.0
95.00	69656.0
96.00	4620.0
103.90	369.0
105.80	373.0
110.90	131.0
115.80	344.0
117.00	550.0
117.80	297.0
118.90	495.0
127.70	305.0
129.00	144.0
129.70	312.0
130.80	151.0
134.90	120.0
136.90	206.0
140.80	1039.0
141.90	125.0
142.90	1161.0
144.90	191.0
145.80	111.0
147.80	182.0
154.90	207.0
156.90	124.0
158.90	134.0
171.80	384.0
173.90	55768.0
174.90	4133.0
175.90	56272.0
176.90	3795.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
35.90	409.0
37.00	2891.0
38.00	2329.0
38.90	989.0
39.90	126.0
43.90	346.0
44.90	436.0
46.90	547.0
47.90	615.0
49.00	3016.0
50.00	12119.0
51.00	3393.0
52.00	200.0
55.00	180.0
55.90	992.0
57.00	1914.0
59.90	804.0
61.00	3660.0
62.00	3742.0
63.00	3319.0
63.90	383.0
64.90	212.0
67.00	234.0
68.00	7285.0
69.00	7339.0
69.90	613.0
71.90	429.0
72.90	3801.0
74.00	13920.0
75.00	40512.0
76.00	3443.0
77.00	422.0
77.90	187.0
78.90	2437.0
79.90	663.0
80.90	2368.0
81.90	617.0
86.00	125.0
86.90	2448.0
87.90	2220.0
90.90	200.0
92.00	2451.0
93.00	3154.0
94.00	9204.0
95.00	71264.0
96.00	4548.0
96.90	103.0
104.00	384.0
105.80	378.0
110.80	108.0
115.80	412.0
117.00	470.0
117.80	331.0
118.90	492.0
127.70	350.0
128.90	119.0
129.80	318.0
130.80	150.0
134.90	103.0
136.90	171.0
140.80	1164.0
141.90	157.0
142.80	1163.0
144.90	168.0
145.80	170.0
147.80	205.0
149.70	125.0
154.90	235.0
156.80	155.0
158.90	151.0
160.60	107.0
171.80	403.0
173.90	58672.0
174.90	4232.0
175.90	58664.0
176.90	3836.0
177.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
35.90	751.0
36.90	3099.0
38.00	2480.0
39.00	994.0
40.10	358.0
40.80	100.0
44.00	1003.0
45.00	656.0
45.90	255.0
47.00	897.0
47.80	430.0
49.00	2427.0
50.00	11126.0
51.00	3394.0
51.90	207.0
52.80	111.0
53.80	109.0
54.80	265.0
56.00	975.0
57.10	1373.0
59.80	617.0
61.00	3112.0
61.90	3222.0
63.00	2476.0
64.00	524.0
64.90	568.0
66.90	232.0
67.90	6022.0
68.90	5735.0
69.80	310.0
72.10	284.0
72.90	2453.0
73.90	9519.0
75.00	28872.0
76.00	2812.0
76.90	463.0
78.00	216.0
78.90	2769.0
79.80	762.0
80.90	2688.0
81.90	572.0
86.90	2469.0
87.90	2192.0
88.80	128.0
90.90	215.0
91.90	1823.0
93.00	2653.0
94.00	6620.0
95.00	55496.0
96.00	3666.0
103.80	214.0
105.70	298.0
115.90	174.0
116.80	622.0
117.90	243.0
118.70	397.0
127.90	134.0
130.00	203.0
130.80	103.0
134.90	190.0
136.70	191.0
140.90	569.0
142.80	1225.0
145.00	629.0
146.00	124.0
154.90	142.0
156.90	130.0
170.70	168.0
171.90	524.0
172.90	410.0
173.90	38920.0
174.90	2825.0
175.90	37528.0
176.90	2638.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062