


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011720\
 Data File : VU036507.D
 Acq On : 17 Jan 2020 09:01
 Operator : JC/MD
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 17 14:05:23 2020

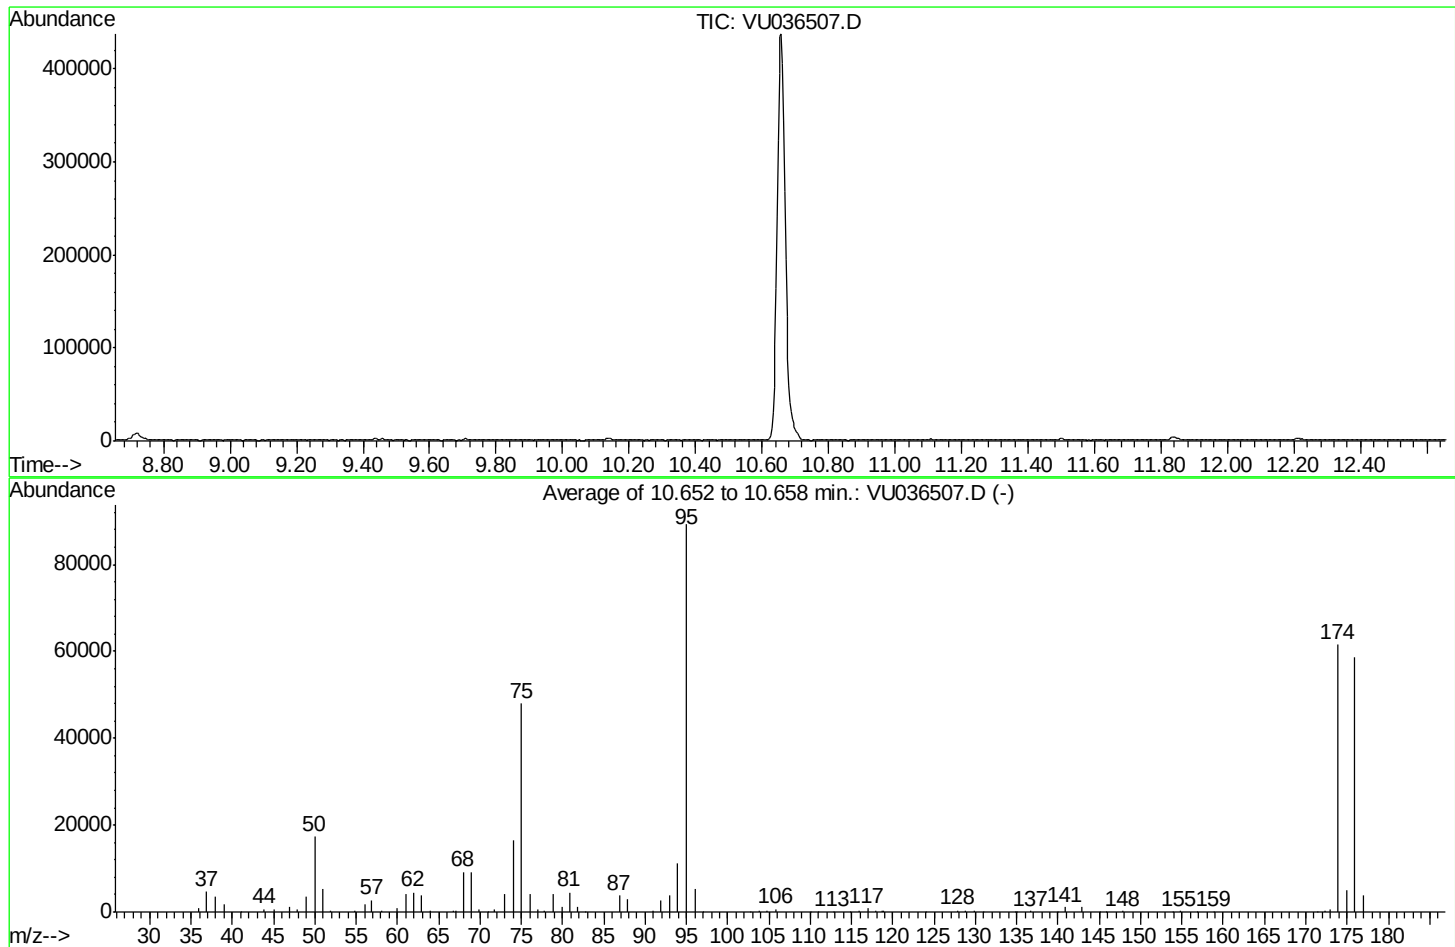

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	17322	PASS
75	95	30	80	53.8	48024	PASS
95	95	100	100	100.0	89232	PASS
96	95	5	9	6.1	5411	PASS
173	174	0.00	2	1.1	699	PASS
174	95	50	120	68.9	61496	PASS
175	174	5	9	8.3	5112	PASS
176	174	95	101	95.2	58517	PASS
177	176	5	9	6.5	3806	PASS

m/z	Abundance
35.90	962.0
36.90	4330.0
37.90	3151.0
38.90	1885.0
41.10	116.0
43.90	1235.0
45.00	609.0
47.00	1152.0
47.80	704.0
48.90	3350.0
49.90	16384.0
51.00	4807.0
51.90	291.0
55.00	374.0
56.00	1898.0
56.90	2560.0
58.10	208.0
59.90	917.0
61.00	4238.0
62.00	4314.0
62.90	3814.0
64.00	385.0
66.80	361.0
67.90	8317.0
69.00	8942.0
69.90	525.0
70.90	149.0
71.80	508.0
72.90	3870.0
74.00	15936.0
75.00	43560.0
76.00	4238.0
76.90	586.0
77.80	141.0
78.80	3919.0
79.90	1026.0
80.90	4008.0
81.80	1139.0
86.90	3193.0
87.90	3123.0
90.90	403.0
92.00	2474.0
92.90	3467.0
94.00	10389.0
95.00	84352.0
96.00	4952.0
97.00	189.0
102.80	114.0
103.70	379.0
104.80	151.0
105.90	534.0
112.90	150.0
114.80	110.0
115.80	297.0
117.00	655.0
117.80	372.0
118.70	461.0
124.00	123.0
127.90	409.0
128.80	192.0
129.80	246.0
130.90	156.0
134.70	150.0
136.70	154.0
140.00	160.0
140.90	916.0
142.90	1103.0
145.00	155.0
147.90	266.0
153.90	117.0
154.80	284.0
156.90	169.0
158.80	120.0
171.40	148.0
172.20	362.0
172.90	581.0
173.90	55432.0
174.90	4719.0
175.90	54416.0
176.90	3627.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	896.0
36.90	4619.0
37.90	3487.0
38.90	1897.0
43.90	1377.0
45.00	593.0
47.00	1165.0
47.80	775.0
48.90	3724.0
49.90	17824.0
51.00	5270.0
51.90	393.0
54.90	372.0
56.00	1882.0
56.90	2776.0
58.10	237.0
59.90	986.0
61.00	4373.0
62.00	4606.0
63.00	4052.0
64.00	264.0
66.70	359.0
67.10	288.0
68.00	9459.0
69.00	9472.0
69.90	599.0
70.90	137.0
71.80	467.0
72.90	4298.0
74.00	17240.0
75.00	49376.0
76.00	4219.0
77.00	557.0
77.80	245.0
78.90	4147.0
79.90	1162.0
80.80	4665.0
81.80	1161.0
86.90	3940.0
87.90	3064.0
90.90	430.0
92.00	2588.0
93.00	3920.0
94.00	11345.0
95.00	92144.0
96.00	5549.0
97.00	137.0
103.70	454.0
104.80	202.0
105.90	616.0
110.00	101.0
110.90	106.0
112.70	141.0
115.80	353.0
117.00	819.0
117.90	451.0
118.70	467.0
127.90	464.0
128.80	275.0
129.80	290.0
130.90	159.0
134.80	118.0
136.70	161.0
140.90	1065.0
142.90	1100.0
145.00	193.0
147.90	332.0
154.80	254.0
156.90	181.0
158.90	113.0
171.40	128.0
172.30	405.0
172.90	695.0
173.90	63352.0
174.90	5301.0
175.90	59616.0
176.90	3917.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	762.0
36.90	4814.0
37.90	3798.0
39.00	1655.0
39.80	164.0
43.90	1316.0
45.00	585.0
47.00	1112.0
47.80	707.0
48.90	3764.0
50.00	17760.0
51.00	5559.0
51.90	390.0
54.80	315.0
56.00	1653.0
56.90	2793.0
58.10	168.0
59.90	833.0
61.00	4016.0
61.90	4508.0
63.00	3924.0
63.90	206.0
66.70	261.0
67.10	215.0
68.00	10031.0
69.00	9236.0
69.90	675.0
71.70	383.0
73.00	4210.0
74.00	16384.0
75.00	51136.0
76.00	3882.0
77.00	509.0
77.80	342.0
78.90	4016.0
79.90	1123.0
80.80	4674.0
81.80	985.0
82.80	159.0
86.90	4081.0
87.90	2921.0
90.90	487.0
91.90	2532.0
92.90	4019.0
93.90	11499.0
95.00	91200.0
96.00	5734.0
96.90	130.0
103.80	497.0
104.80	222.0
105.90	655.0
110.90	100.0
112.70	118.0
115.90	418.0
116.90	959.0
118.00	500.0
118.90	501.0
127.80	446.0
128.80	250.0
129.80	317.0
130.90	135.0
135.00	112.0
136.70	173.0
140.90	1254.0
143.00	1004.0
145.00	131.0
145.80	118.0
147.90	270.0
154.80	170.0
156.90	112.0
159.00	132.0
172.90	823.0
173.90	65704.0
174.90	5317.0
175.90	61520.0
176.90	3874.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Scan 2884 (10.613 min): VU036507.D
BFB42

m/z	Abundance
39.80	272.0
42.80	180.0
43.90	648.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42