




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052717.D
 Acq On : 17 Jan 2023 13:26
 Operator : JC/MD
 Sample : 01138-20DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Y3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:17:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 18 01:16:13 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/20/2023
 Supervised By :Mahesh Dadoda 01/20/2023

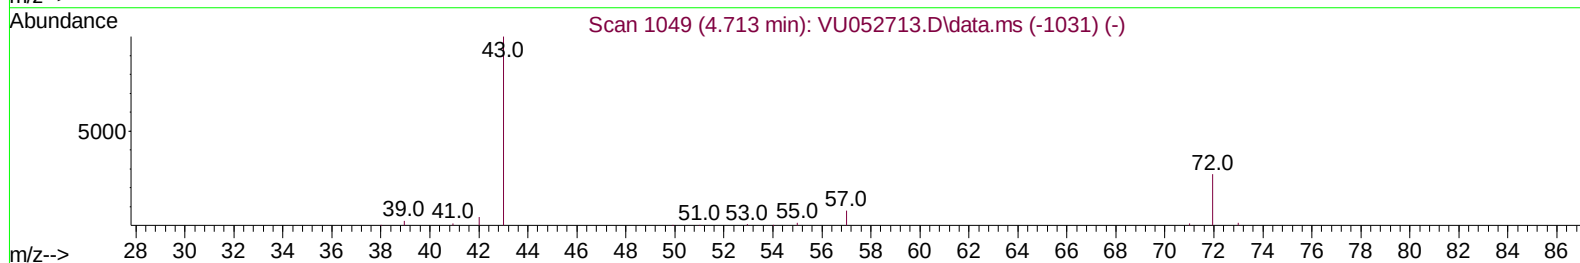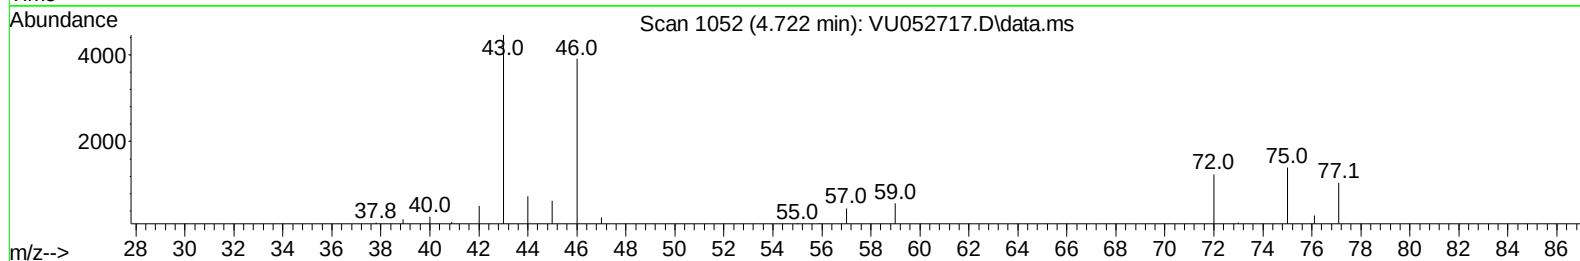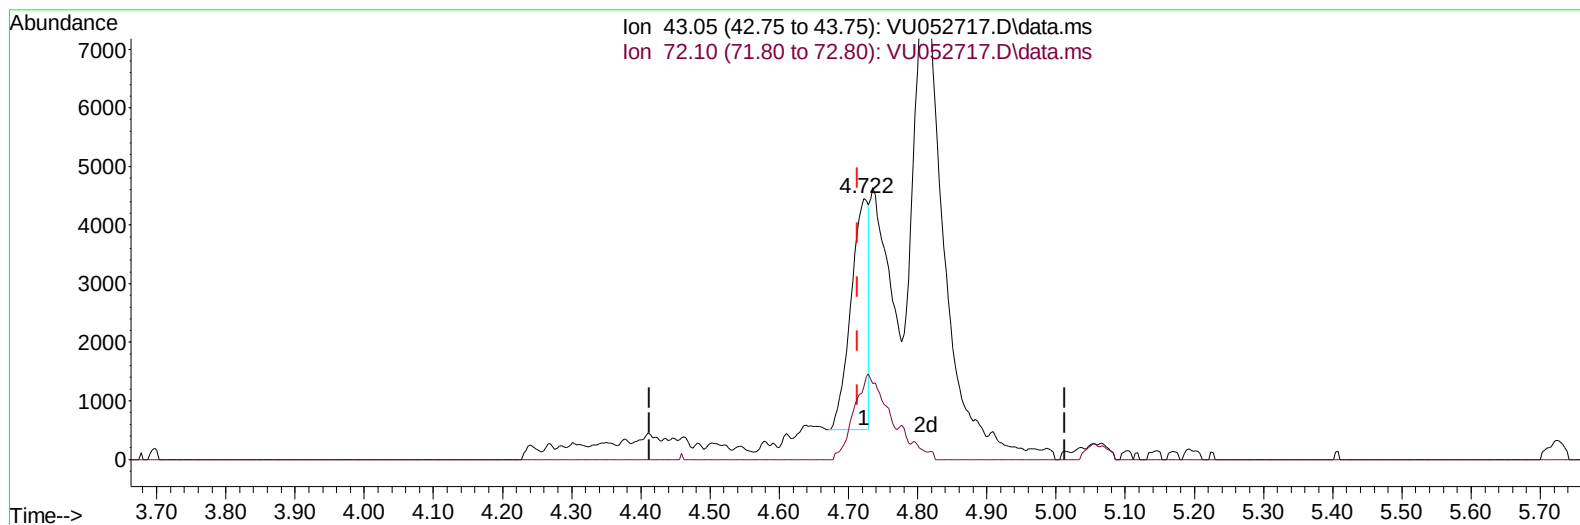

TIC: VU052717.D\data.ms

(21) 2-Butanone (T)

4.722min (+ 0.010) 2.04 ug/L

response 6986

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.70	65.80#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052717.D
 Acq On : 17 Jan 2023 13:26
 Operator : JC/MD
 Sample : 01138-20DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Y3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:17:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 18 01:16:13 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/20/2023
 Supervised By :Mahesh Dadoda 01/20/2023

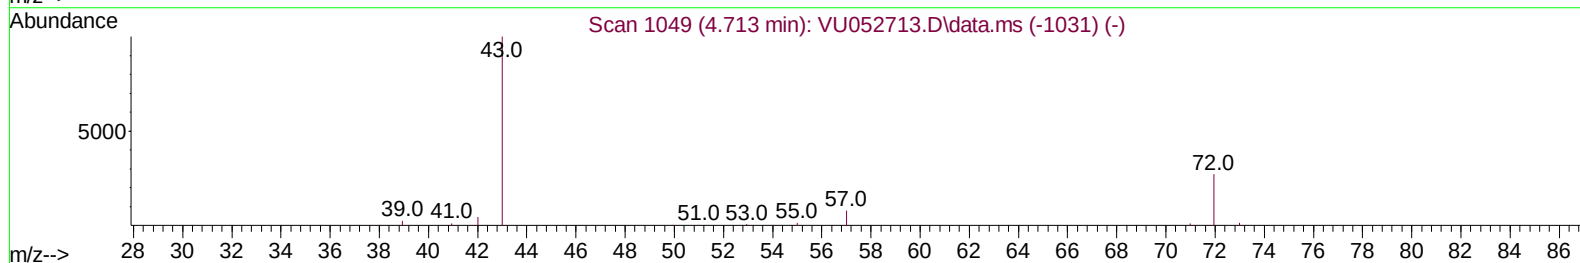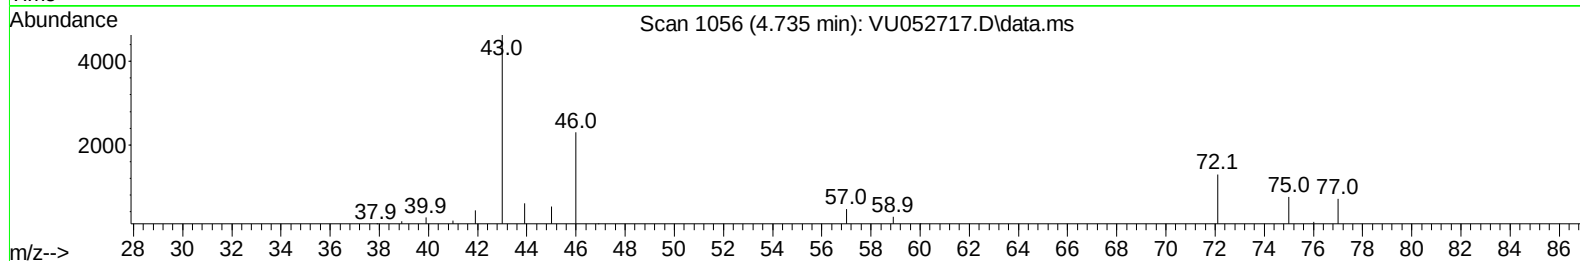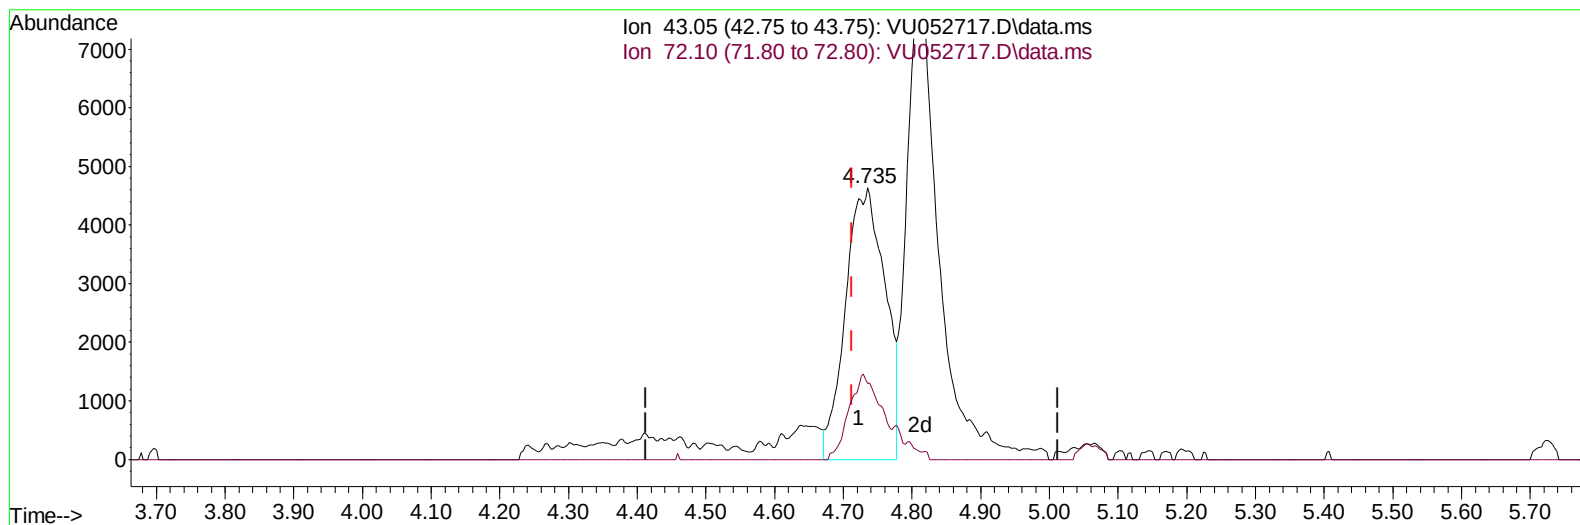

TIC: VU052717.D\data.ms

(21) 2-Butanone (T)

4.735min (+ 0.022) 5.39 ug/L m

response 18484

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.70	24.87
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052717.D
 Acq On : 17 Jan 2023 13:26
 Operator : JC/MD
 Sample : 01138-20DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Y3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:17:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 18 01:16:13 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 01/20/2023
 Supervised By :Mahesh Dadoda 01/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	126506	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	122636	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	53633	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50894	4.579	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	91.600%		
7) Chloroethane-d5	1.912	69	44833	4.951	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.000%		
11) 1,1-Dichloroethene-d2	2.565	65	24537	5.013	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	100.200%		
20) 2-Butanone-d5	4.642	46	145870	49.087	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	98.180%		
24) Chloroform-d	5.057	84	110075	5.309	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	106.200%		
26) 1,2-Dichloroethane-d4	5.697	65	57737	5.423	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	108.400%		
32) Benzene-d6	5.722	84	217114	5.462	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	109.200%		
36) 1,2-Dichloropropane-d6	6.687	67	69120	5.218	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	104.400%		
41) Toluene-d8	7.893	98	179548	5.123	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.400%		
43) trans-1,3-Dichloroprop...	8.176	79	23513	4.773	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	95.400%		
46) 2-Hexanone-d5	8.632	63	105120	51.373	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	102.740%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	51468	5.075	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.400%		
66) 1,2-Dichlorobenzene-d4	12.188	152	60056	6.151	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	123.000%#		
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.575	96	6749	0.615	ug/L #	1
16) Methylene chloride	3.044	84	5587	0.383	ug/L	88
19) 1,1-Dichloroethane	3.861	63	4541	0.196	ug/L	96
21) 2-Butanone	4.735	43	18484m	5.388	ug/L	
22) cis-1,2-Dichloroethene	4.661	96	11831	0.985	ug/L	96
34) Trichloroethene	6.539	95	130564	11.371	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052717.D
Acq On : 17 Jan 2023 13:26
Operator : JC/MD
Sample : 01138-20DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Y3DL

Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:17:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 18 01:16:13 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 01/20/2023
Supervised By :Mahesh Dadoda 01/20/2023

