

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052723.D
 Acq On : 17 Jan 2023 15:57
 Operator : JC/MD
 Sample : 01138-16 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1X9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	96	rBV	73360	89345	15.02%	1.942%
2	1.916	170	179	196	rVB	57820	79382	13.34%	1.726%
3	2.565	368	381	395	rBV	127973	208271	35.01%	4.527%
4	2.790	439	451	466	rBV	8425	14268	2.40%	0.310%
5	3.041	518	529	542	rBV3	8879	17029	2.86%	0.370%
6	3.179	555	572	586	rBV2	2716	6245	1.05%	0.136%
7	4.642	1010	1027	1062	rBV	77681	277348	46.62%	6.029%
8	5.057	1140	1156	1178	rBV2	116034	259918	43.69%	5.650%
9	5.723	1338	1363	1382	rBV3	227867	594928	100.00%	12.933%
10	6.243	1512	1525	1543	rBV	152350	288115	48.43%	6.263%
11	6.539	1605	1617	1631	rVB3	31729	58613	9.85%	1.274%
12	6.687	1649	1663	1685	rVB	146276	283505	47.65%	6.163%
13	7.562	1923	1935	1951	rBV	65886	114740	19.29%	2.494%
14	7.893	2025	2038	2055	rBV	264207	457762	76.94%	9.951%
15	8.176	2113	2126	2141	rBV	40912	68769	11.56%	1.495%
16	8.632	2254	2268	2300	rBV2	302367	580683	97.61%	12.623%
17	9.414	2495	2511	2532	rBV	220303	358679	60.29%	7.797%
18	10.751	2915	2927	2941	rBV	105860	166958	28.06%	3.629%
19	11.806	3244	3255	3274	rBV	195384	311513	52.36%	6.772%
20	12.189	3361	3374	3392	rBV	226209	364123	61.20%	7.915%




Sum of corrected areas: 4600194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052723.D
Acq On : 17 Jan 2023 15:57
Operator : JC/MD
Sample : 01138-16 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

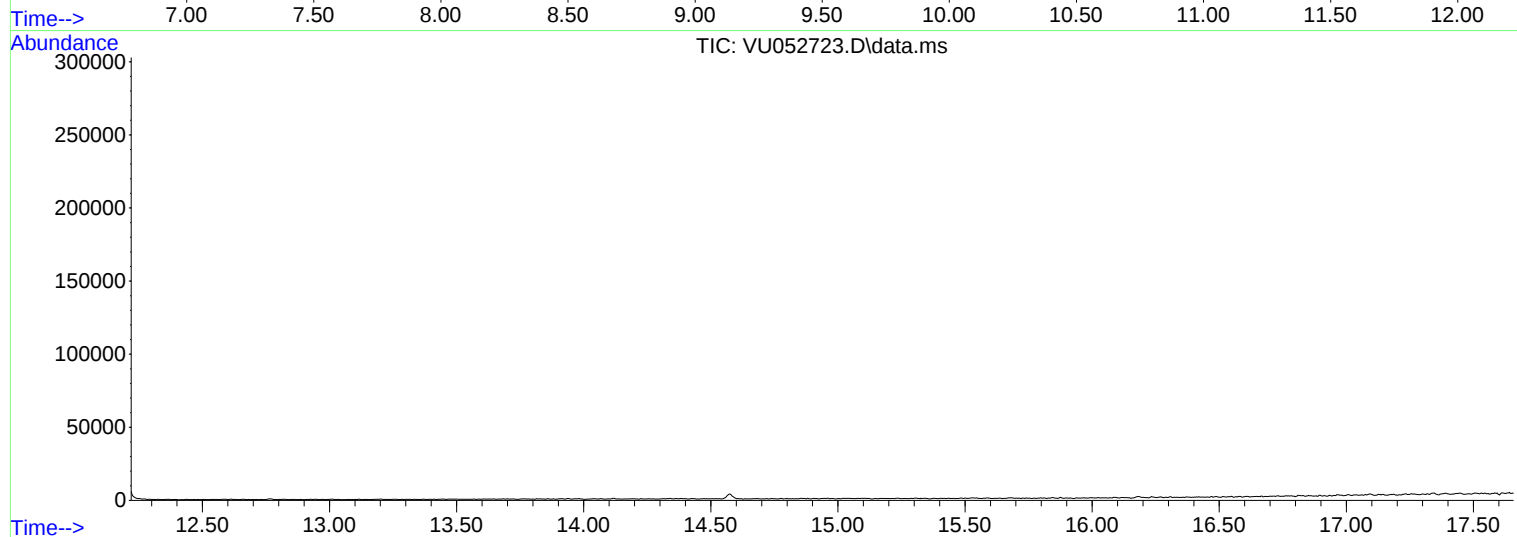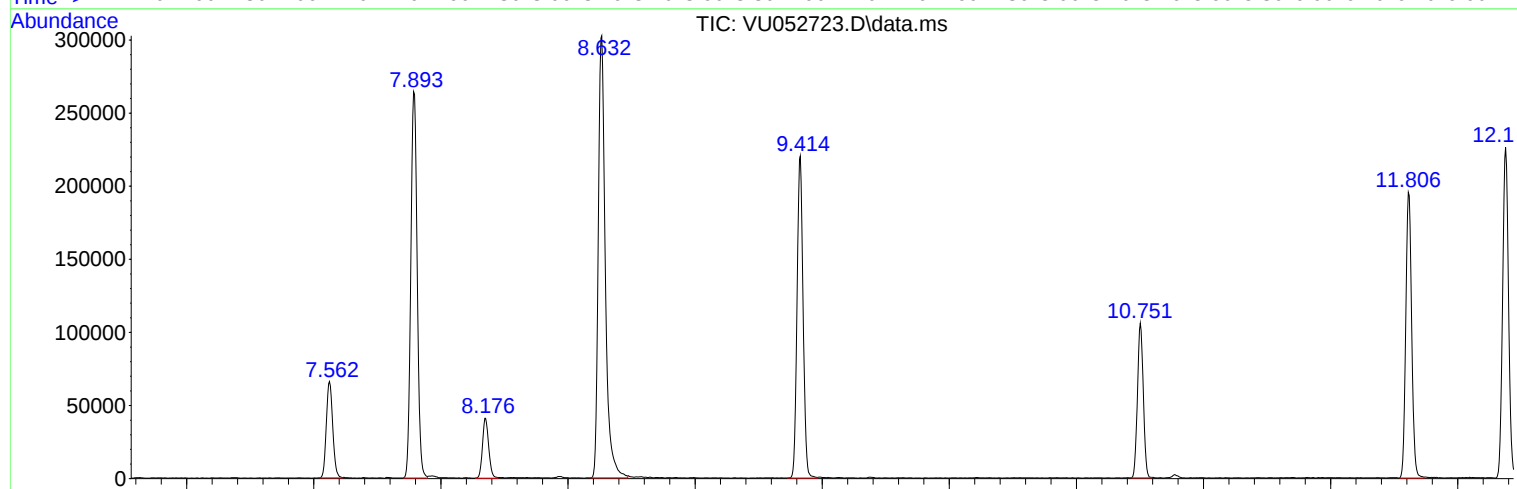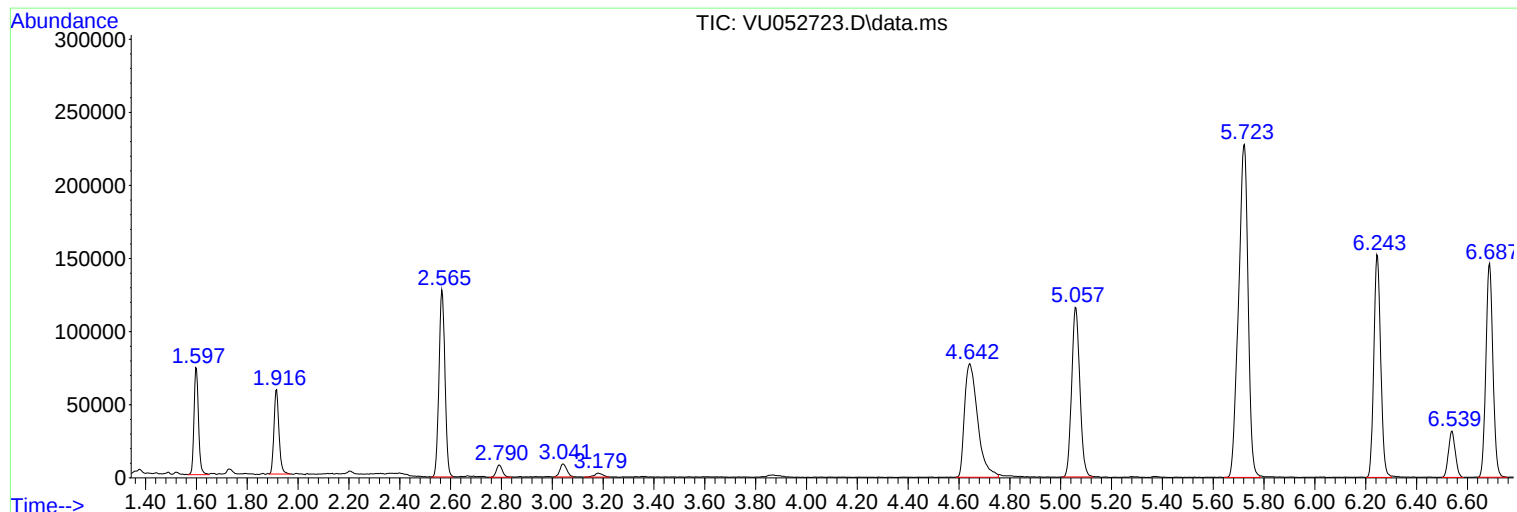

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052723.D
Acq On : 17 Jan 2023 15:57
Operator : JC/MD
Sample : 01138-16 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052723.D
Acq On : 17 Jan 2023 15:57
Operator : JC/MD
Sample : 01138-16 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc