

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052727.D
 Acq On : 17 Jan 2023 17:36
 Operator : JC/MD
 Sample : 01136-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	62681	73112	13.39%	1.720%
2	1.916	169	179	197	rVB	53951	75593	13.85%	1.778%
3	2.565	366	381	399	rBV	121075	198572	36.37%	4.671%
4	2.793	439	452	463	rBV	7097	12756	2.34%	0.300%
5	3.044	518	530	546	rVB3	15282	29186	5.35%	0.686%
6	4.639	1011	1026	1053	rBV	63876	216562	39.67%	5.094%
7	5.057	1140	1156	1180	rBV	107627	241620	44.26%	5.683%
8	5.723	1341	1363	1387	rBV3	211714	545718	99.96%	12.836%
9	6.243	1512	1525	1547	rBV	157845	295708	54.17%	6.955%
10	6.687	1646	1663	1685	rBV	133552	261307	47.87%	6.146%
11	7.562	1922	1935	1953	rBV	60021	105023	19.24%	2.470%
12	7.893	2022	2038	2057	rBV	244421	417158	76.41%	9.812%
13	8.176	2113	2126	2141	rBV2	36489	62889	11.52%	1.479%
14	8.632	2255	2268	2301	rBV2	283720	545922	100.00%	12.840%
15	9.414	2498	2511	2530	rBV	222444	364288	66.73%	8.568%
16	10.751	2915	2927	2941	rBV	96806	154247	28.25%	3.628%
17	11.809	3241	3256	3275	rBV	192024	310014	56.79%	7.292%
18	12.189	3361	3374	3395	rBV	209419	333382	61.07%	7.841%
19	14.574	4105	4116	4128	rBV2	4979	8531	1.56%	0.201%




Sum of corrected areas: 4251588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052727.D
Acq On : 17 Jan 2023 17:36
Operator : JC/MD
Sample : 01136-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

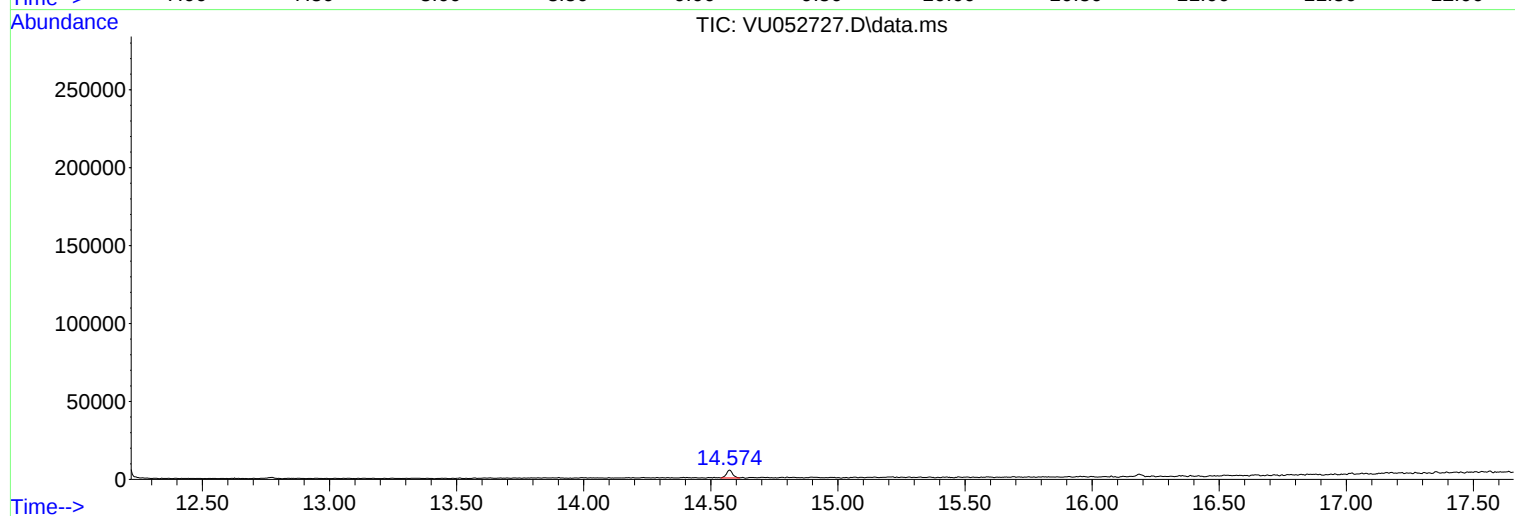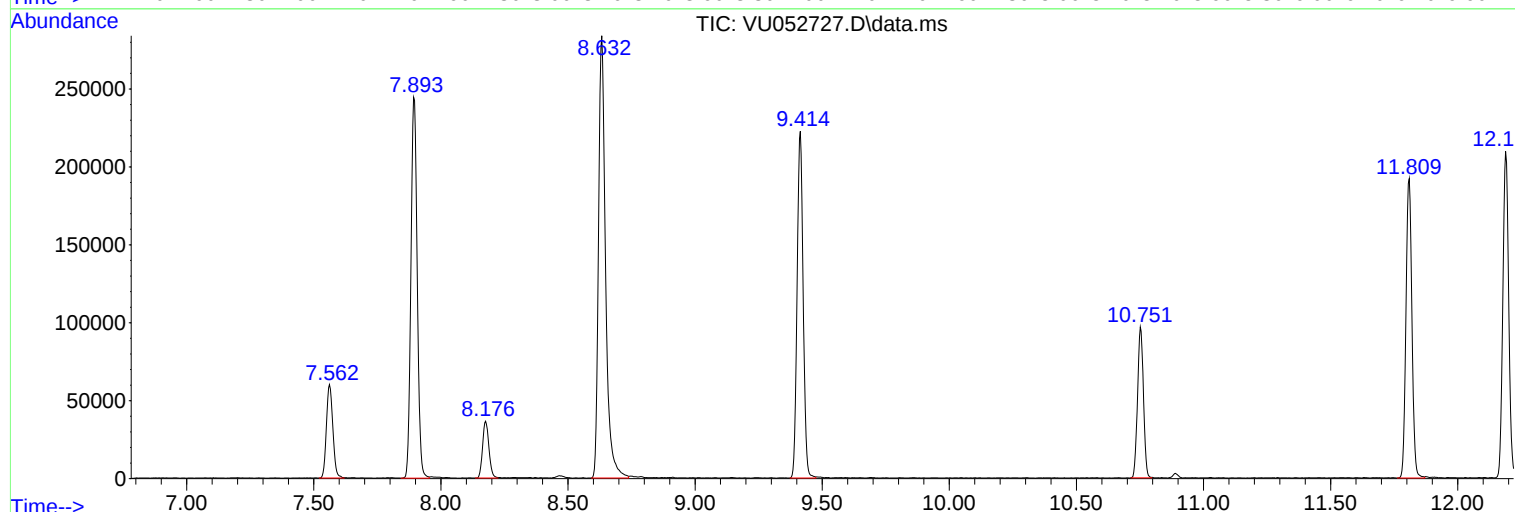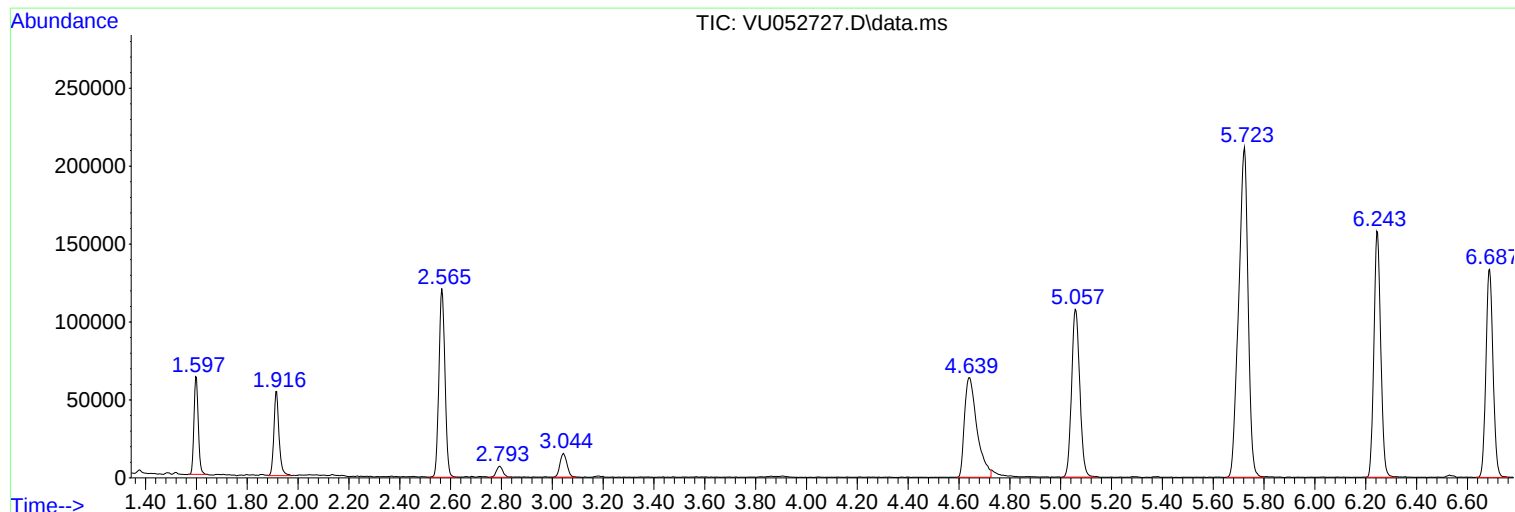

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052727.D
Acq On : 17 Jan 2023 17:36
Operator : JC/MD
Sample : 01136-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
Data File : VU052727.D
Acq On : 17 Jan 2023 17:36
Operator : JC/MD
Sample : 01136-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc