
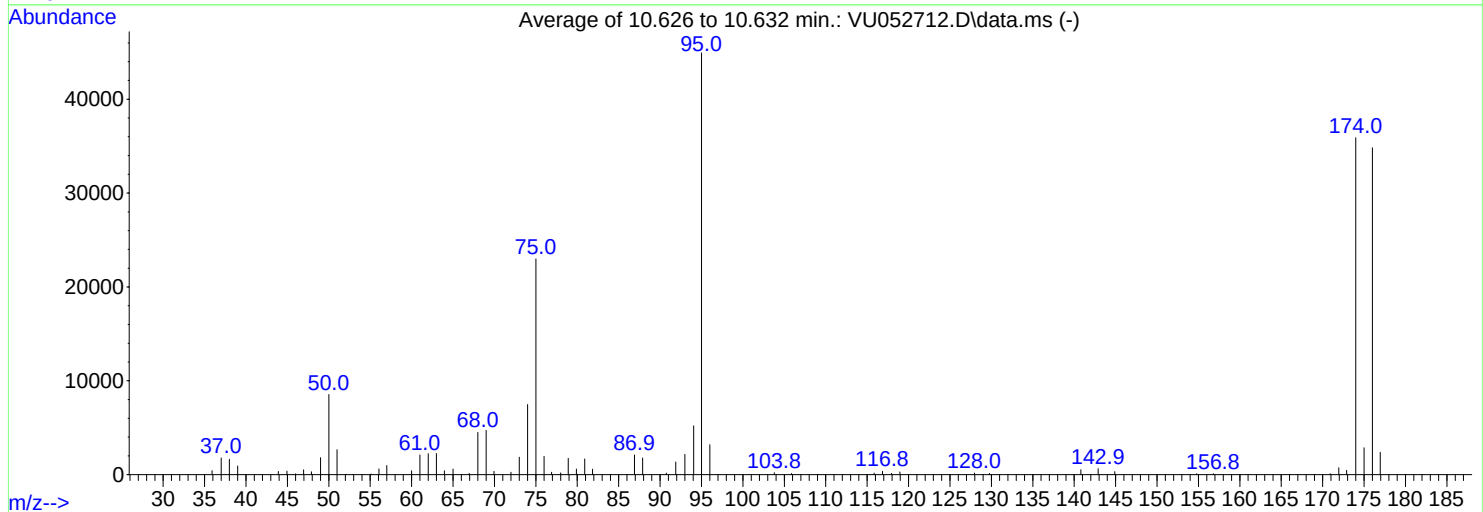


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011723\
 Data File : VU052712.D
 Acq On : 17 Jan 2023 09:41
 Operator : JC/MD
 Sample : BFB191
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB191

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 18 01:16:13 2023

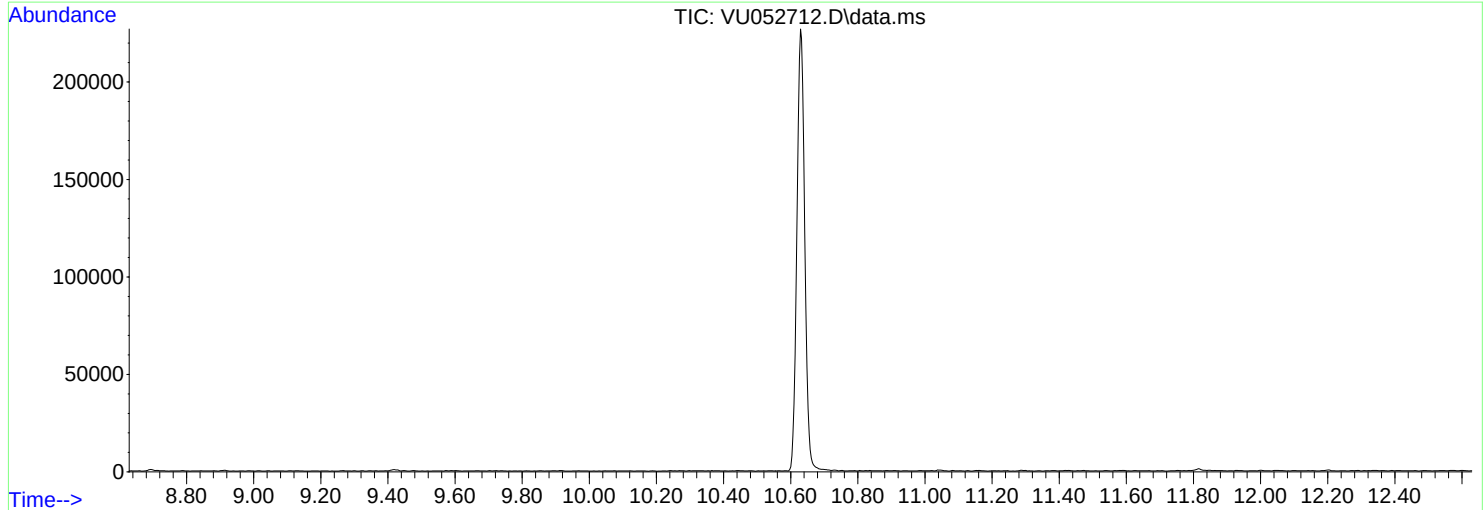

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	8551	PASS
75	95	30	80	51.1	22987	PASS
95	95	100	100	100.0	44944	PASS
96	95	5	9	7.1	3182	PASS
173	174	0.00	2	1.3	457	PASS
174	95	50	120	79.9	35907	PASS
175	174	5	9	8.0	2861	PASS
176	174	95	101	97.0	34824	PASS
177	176	5	9	6.9	2392	PASS

m/z	Abundance
39.90	387.0
43.80	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
35.90	425.0
37.00	1674.0
38.00	1492.0
39.00	878.0
39.90	308.0
43.90	503.0
44.90	378.0
46.00	135.0
46.90	478.0
47.90	272.0
49.00	1873.0
50.00	7932.0
51.00	2587.0
52.10	101.0
52.90	109.0
56.00	627.0
57.00	1024.0
60.00	416.0
61.00	2056.0
62.00	2196.0
63.00	1974.0
64.00	484.0
65.00	518.0
67.10	142.0
68.00	4435.0
69.00	4560.0
70.00	378.0
72.00	284.0
73.00	1832.0
74.00	7402.0
75.00	22352.0
76.00	1878.0
76.90	285.0
78.00	192.0
78.90	1672.0
79.90	556.0
80.90	1477.0
81.90	519.0
86.90	2162.0
87.90	1625.0
90.70	169.0
91.90	1243.0
93.00	2013.0
94.00	4969.0
95.00	43736.0
96.00	3010.0
103.80	179.0
105.90	126.0
115.80	190.0
116.80	304.0
118.00	130.0
118.90	256.0
127.90	179.0
129.70	141.0
140.80	533.0
142.90	613.0
144.90	335.0
156.80	156.0
171.90	676.0
172.80	434.0
174.00	33488.0
175.00	2734.0
176.00	33520.0
176.90	2265.0
178.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
35.90	459.0
37.00	1833.0
38.00	1705.0
39.00	988.0
39.90	324.0
44.00	502.0
45.00	408.0
46.00	129.0
47.00	521.0
47.90	318.0
49.00	1876.0
50.00	8871.0
51.00	2790.0
55.10	100.0
56.00	599.0
57.00	986.0
60.00	443.0
61.00	2148.0
62.00	2282.0
63.00	2323.0
64.00	395.0
65.00	605.0
66.90	129.0
68.00	4609.0
69.00	4875.0
70.00	365.0
72.00	269.0
73.00	1844.0
74.00	7790.0
75.00	23728.0
76.00	2056.0
76.90	243.0
78.00	198.0
78.90	1767.0
79.90	633.0
80.90	1740.0
81.80	606.0
86.90	2229.0
87.90	1804.0
90.80	171.0
91.90	1374.0
93.00	2244.0
94.00	5297.0
95.00	46152.0
96.00	3308.0
103.80	208.0
105.90	121.0
115.80	171.0
116.90	360.0
117.90	143.0
118.90	299.0
127.90	177.0
129.80	136.0
140.80	560.0
142.90	660.0
144.90	335.0
154.80	131.0
156.80	144.0
170.90	130.0
171.90	743.0
172.90	455.0
174.00	37056.0
175.00	2976.0
176.00	35872.0
177.00	2461.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191

m/z	Abundance
35.90	408.0
37.00	1831.0
38.00	1728.0
39.00	913.0
39.90	353.0
44.00	548.0
45.00	370.0
47.00	550.0
47.90	329.0
49.00	1678.0
50.00	8851.0
51.00	2582.0
55.10	126.0
56.10	602.0
57.00	929.0
60.00	386.0
61.00	2087.0
62.00	2220.0
63.00	2448.0
63.90	372.0
65.00	651.0
66.80	161.0
68.00	4473.0
69.00	4759.0
69.90	346.0
72.00	226.0
73.00	1922.0
74.00	7217.0
75.00	22880.0
76.00	1888.0
76.90	221.0
78.00	157.0
78.90	1761.0
79.90	590.0
80.90	1799.0
81.80	594.0
86.90	1887.0
87.90	1889.0
90.80	176.0
91.90	1435.0
93.00	2253.0
94.10	5316.0
95.00	44944.0
96.00	3229.0
103.80	211.0
105.80	126.0
115.90	136.0
116.90	391.0
117.90	132.0
119.00	292.0
128.00	175.0
129.80	143.0
140.80	516.0
142.90	628.0
144.90	312.0
154.80	163.0
170.90	158.0
172.00	759.0
173.00	481.0
174.00	37176.0
175.00	2873.0
176.00	35080.0
176.90	2449.0

Instrument :
MSVOA_U
ClientSampleId :
BFB191