

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011725\
 Data File : VU062874.D
 Acq On : 17 Jan 2025 16:13
 Operator : MD/SY
 Sample : Q1071-08DL 2X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ74DL

Quant Time: Jan 17 22:00:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 17 21:53:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	85766	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.405	117	79489	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38902	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	20356	4.285	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.800%
7) Chloroethane-d5	1.901	69	18304	4.790	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.800%
11) 1,1-Dichloroethene-d2	2.554	65	11122	4.520	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.400%
20) 2-Butanone-d5	4.605	46	59599	61.390	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.780%
24) Chloroform-d	5.049	84	58729	5.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.689	65	35422	5.588	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.800%
32) Benzene-d6	5.714	84	96436	4.963	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	6.679	67	27045	5.020	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.888	98	88312	4.665	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	8.171	79	13603	5.065	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.400%
46) 2-Hexanone-d5	8.621	63	49277	58.344	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.680%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	25373	5.624	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.400%
66) 1,2-Dichlorobenzene-d4	12.183	152	34844	5.384	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds					Qvalue	
13) Acetone	2.611	43	78735	102.378	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011725\
Data File : VU062874.D
Acq On : 17 Jan 2025 16:13
Operator : MD/SY
Sample : Q1071-08DL 2X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCQ74DL


Quant Time: Jan 17 22:00:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 17 21:53:56 2025
Response via : Initial Calibration

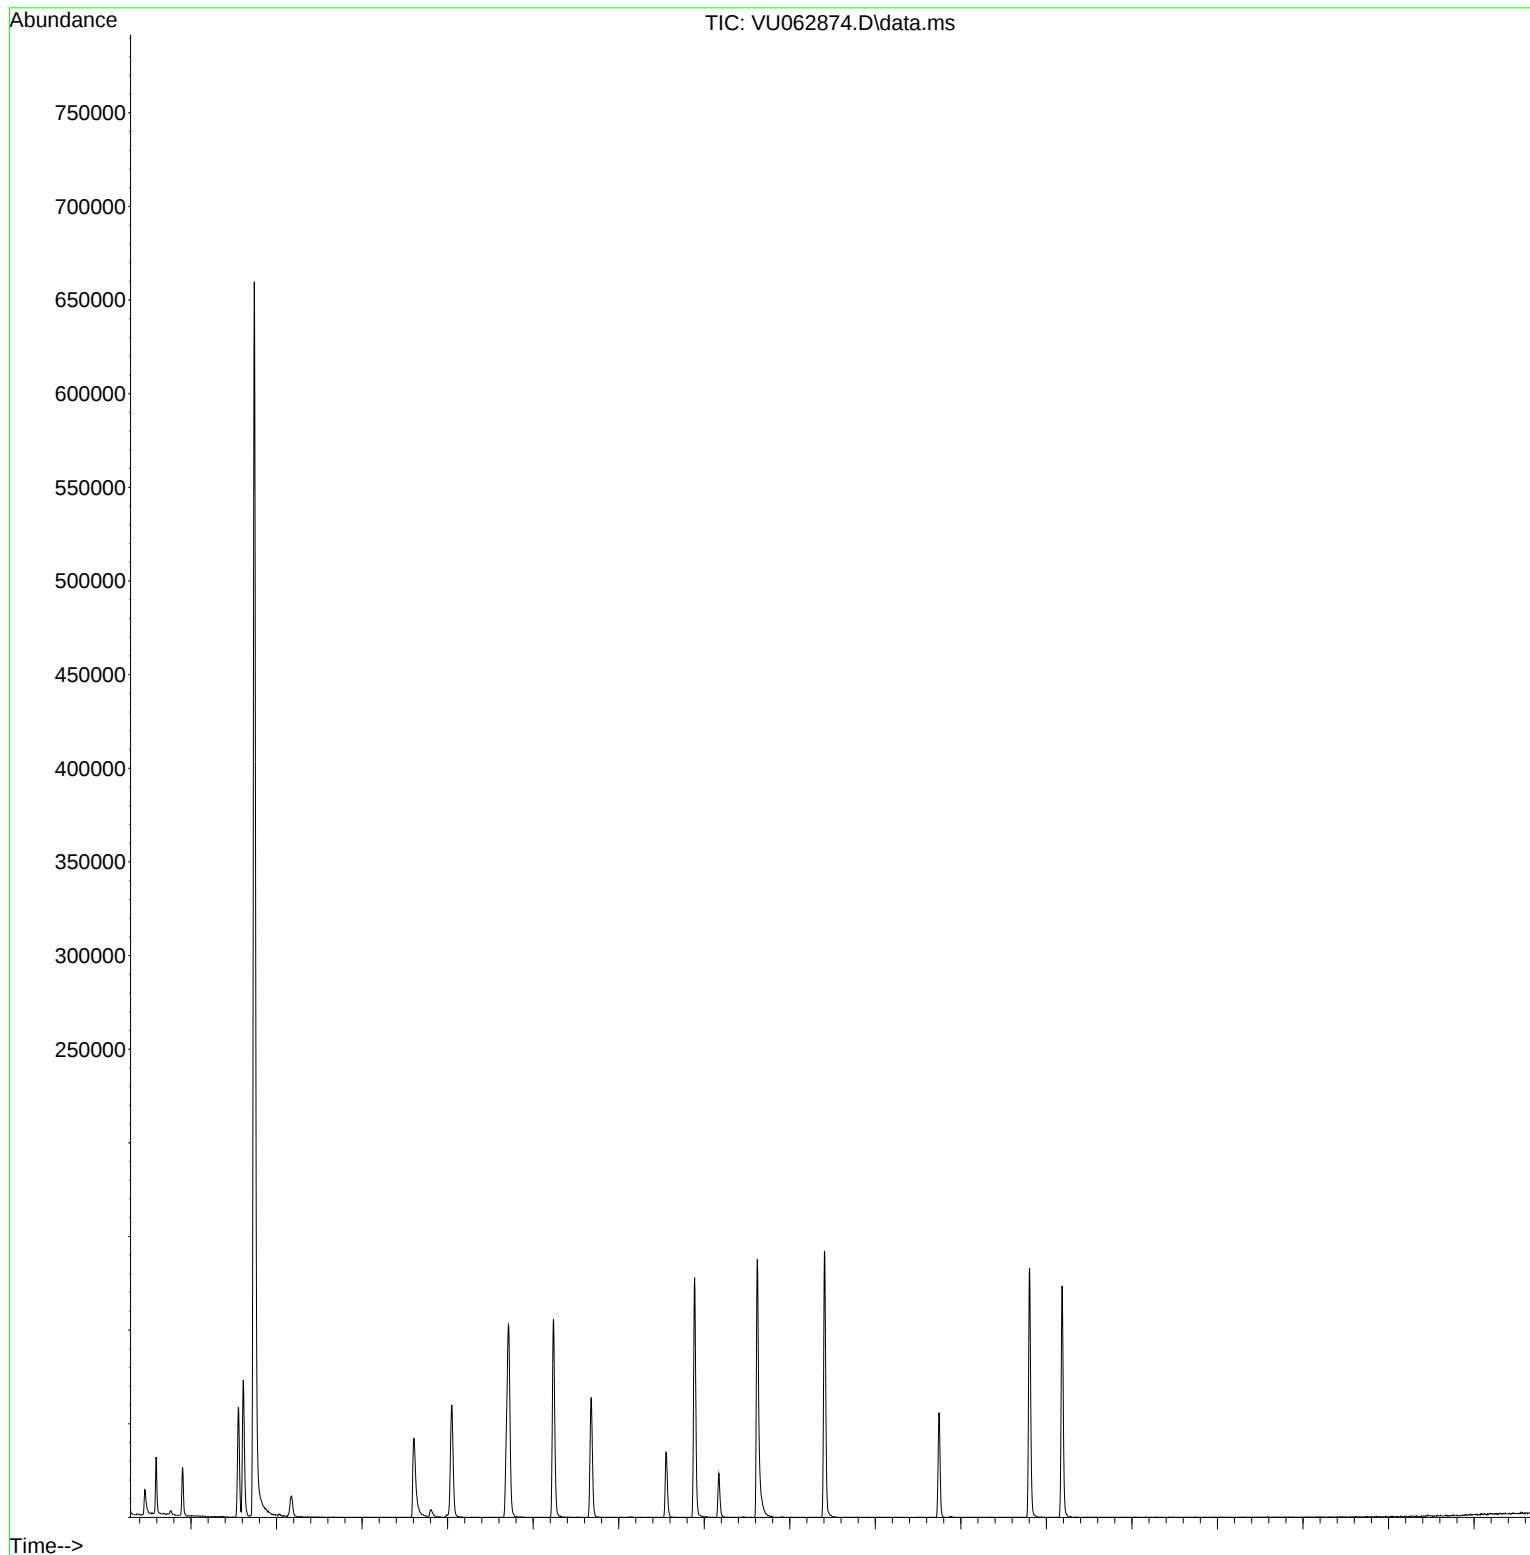

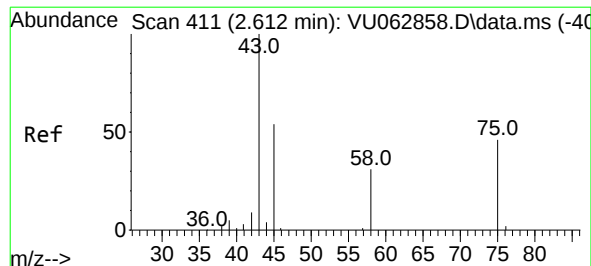

#13
 Acetone
 Concen: 102.378 ug/L
 RT: 2.611 min Scan# 411
 Delta R.T. -0.000 min
 Lab File: VU062874.D
 Acq: 17 Jan 2025 16:13

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ74DL

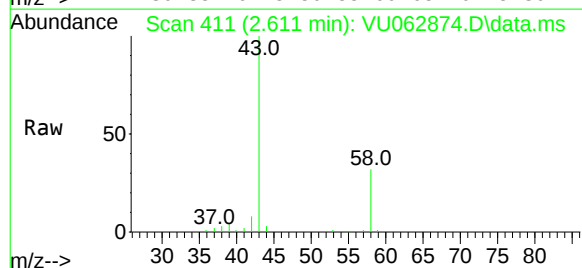

Tgt Ion: 43 Resp: 78735
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 64.4

