

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011725\
 Data File : VU062904.D
 Acq On : 18 Jan 2025 04:56
 Operator : MD/SY
 Sample : VIBLK198
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK198

Quant Time: Jan 18 05:13:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 17 23:41:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	84609	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	80037	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	37357	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	19120	4.080	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.904	69	18172	4.821	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	2.557	65	10329	4.255	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.000%
20) 2-Butanone-d5	4.605	46	47543	49.642	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.280%
24) Chloroform-d	5.049	84	57027	4.946	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.692	65	33325	5.329	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.714	84	92824	4.744	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.679	67	27234	5.021	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.888	98	82372	4.321	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%
43) trans-1,3-Dichloroprop...	8.171	79	12444	4.602	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.000%
46) 2-Hexanone-d5	8.621	63	40831	48.013	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.020%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	24050	5.294	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.800%
66) 1,2-Dichlorobenzene-d4	12.184	152	31685	5.098	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds					Qvalue	
29) 1,1,1-Trichloroethane	5.303	97	8151	0.671	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011725\
Data File : VU062904.D
Acq On : 18 Jan 2025 04:56
Operator : MD/SY
Sample : VIBLK198
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK198


Quant Time: Jan 18 05:13:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 17 23:41:19 2025
Response via : Initial Calibration

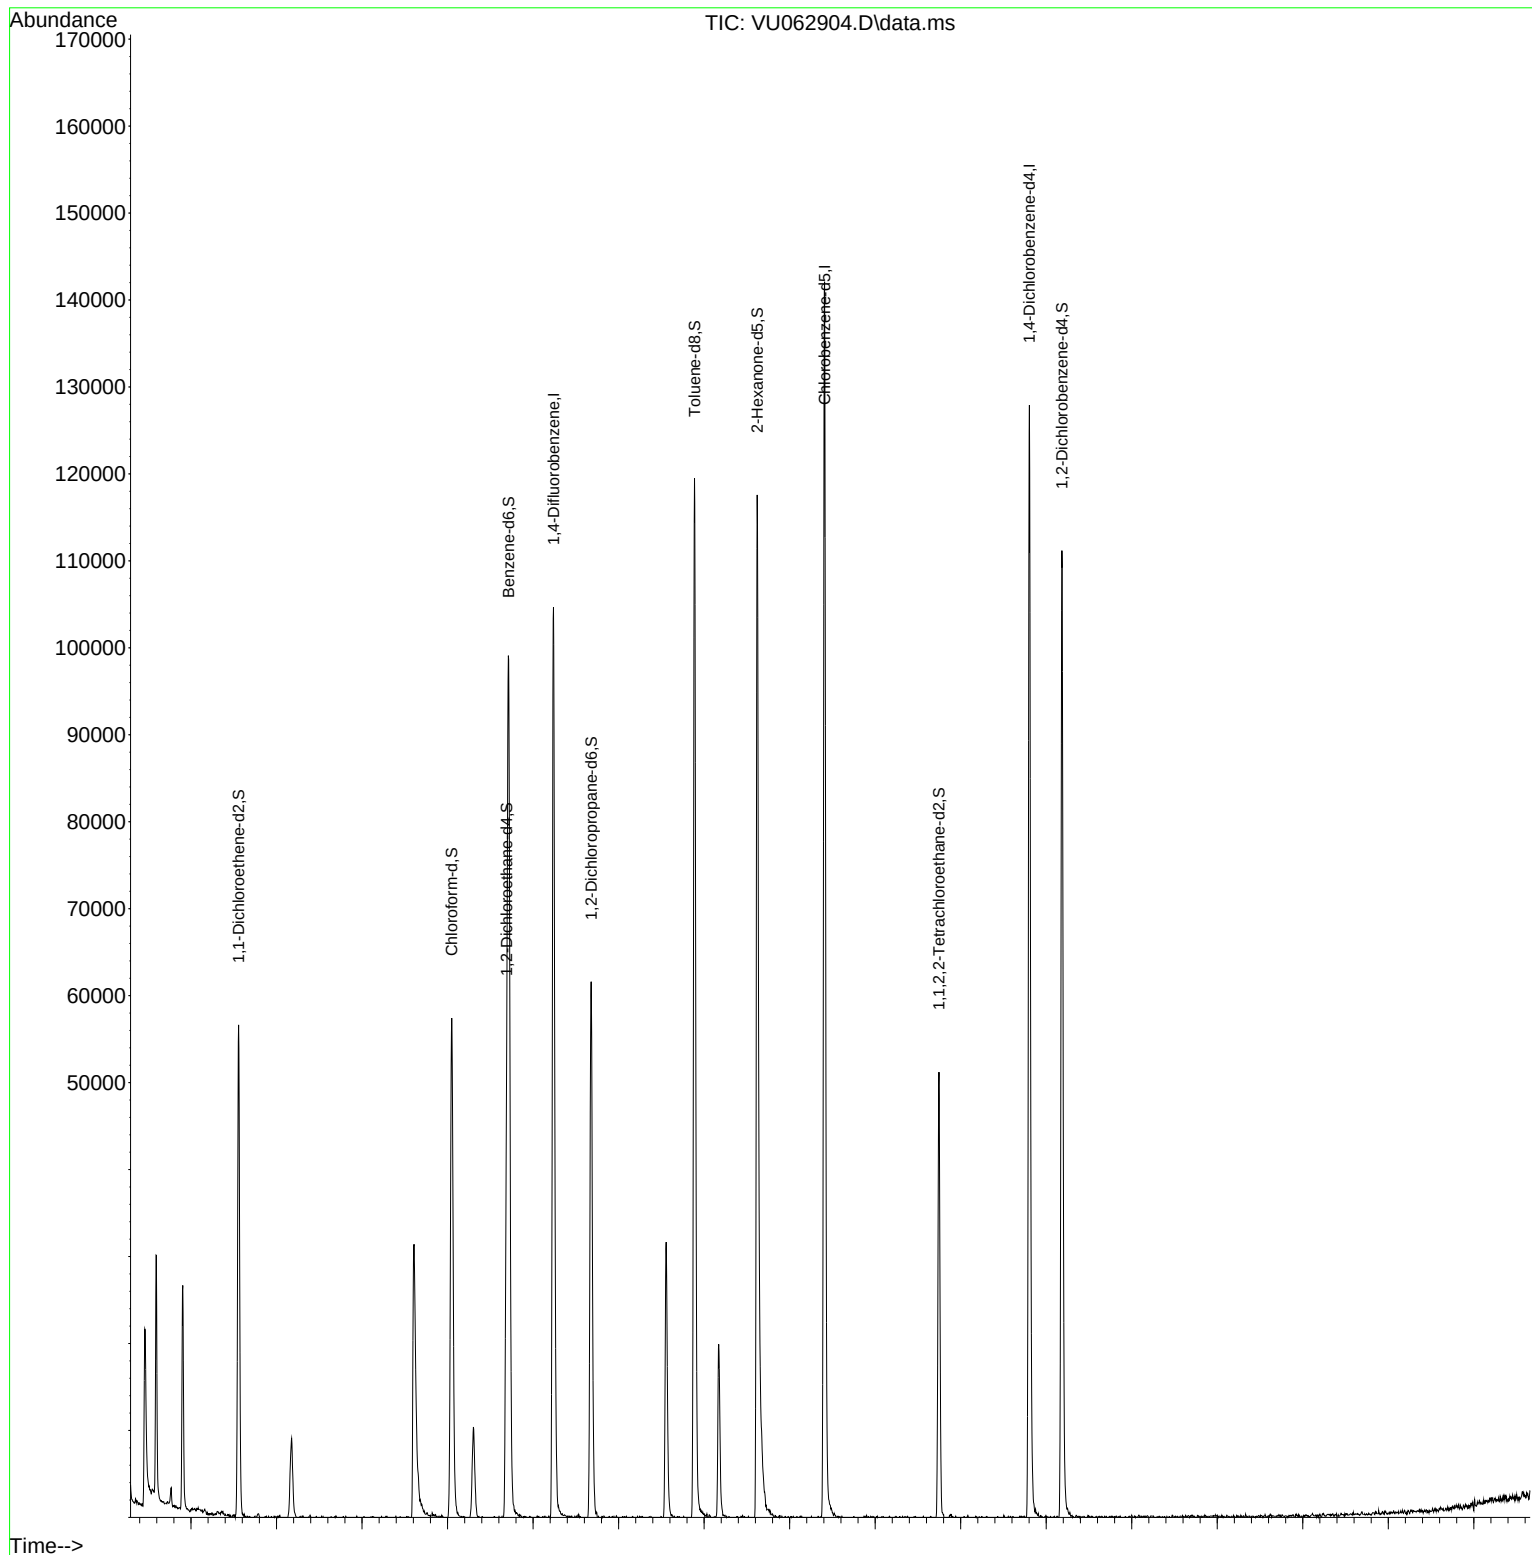

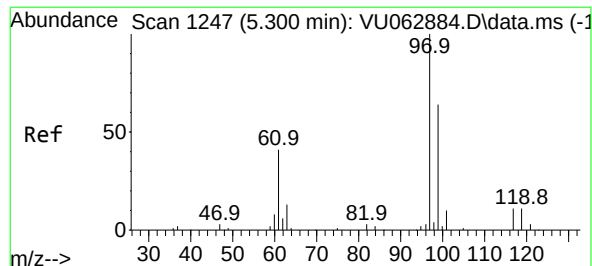

1,1,1-Trichloroethane
 Concen: 0.671 ug/L
 RT: 5.303 min Scan# 12
 Delta R.T. 0.003 min
 Lab File: VU062904.D
 Acq: 18 Jan 2025 04:56

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK198

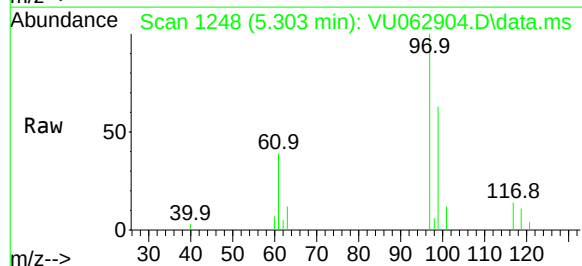

Tgt Ion:	97	Resp:	8151
Ion	Ratio	Lower	Upper
97	100		
99	62.1	52.4	78.6
61	40.1	32.2	48.4

