
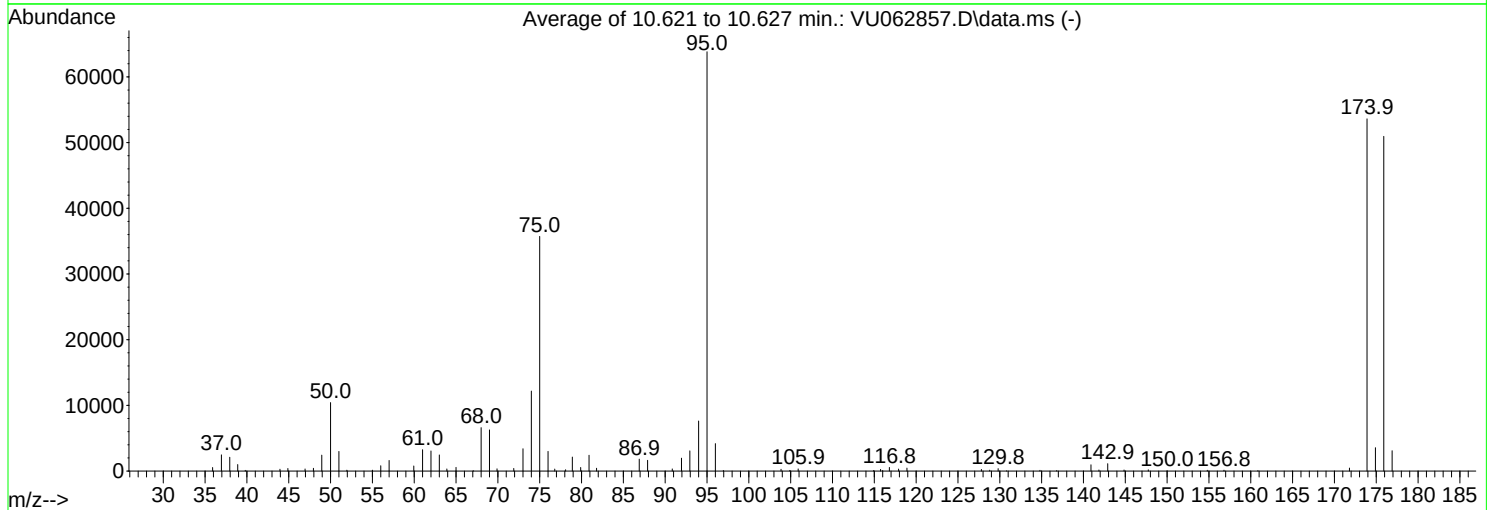


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011725\
Data File : VU062857.D
Acq On : 17 Jan 2025 08:43
Operator : MD/SY
Sample : BFB063
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB063

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 21 02:39:03 2025

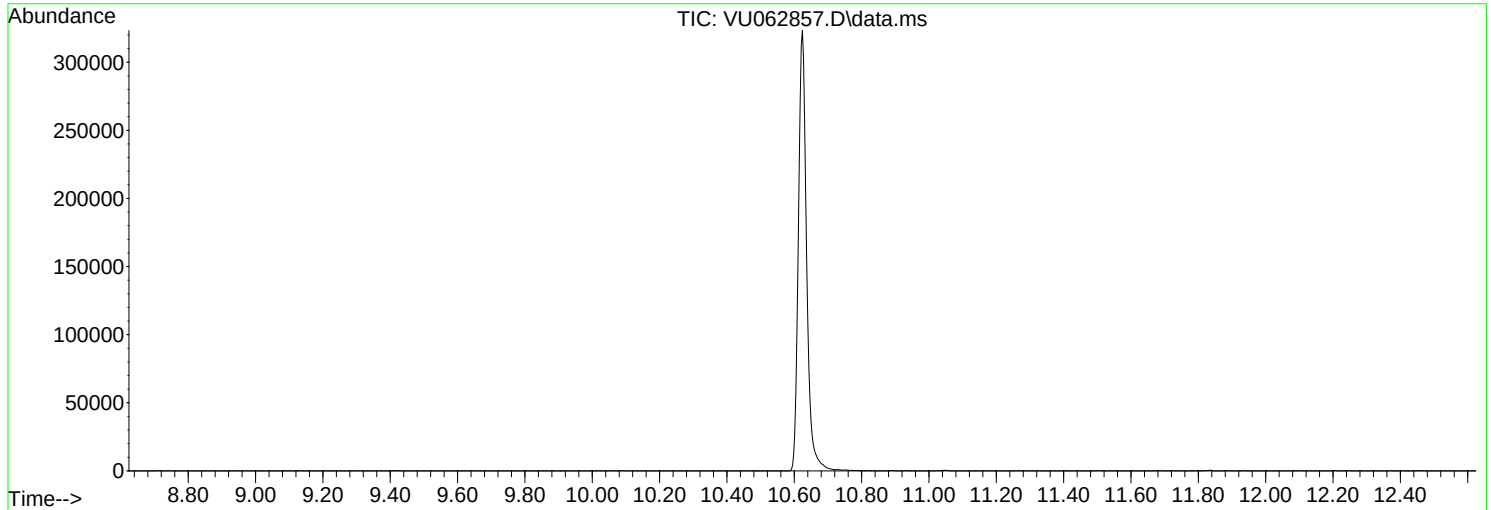

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10430	PASS
75	95	30	80	56.0	35720	PASS
95	95	100	100	100.0	63829	PASS
96	95	5	9	6.5	4177	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	53619	PASS
175	174	5	9	6.6	3560	PASS
176	174	95	101	95.0	50949	PASS
177	176	5	9	6.1	3098	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB063

m/z	Abundance
35.90	520.0
37.00	2586.0
38.00	2115.0
38.90	971.0
39.80	105.0
44.00	322.0
44.90	411.0
47.00	345.0
48.00	432.0
48.90	2379.0
50.00	10466.0
51.00	3282.0
52.00	104.0
54.90	144.0
56.00	808.0
57.00	1649.0
59.90	744.0
61.00	3339.0
62.00	3164.0
63.00	2489.0
63.90	375.0
65.00	507.0
68.00	6506.0
69.00	6350.0
69.90	387.0
71.00	413.0
73.90	3422.0
74.00	12283.0
75.00	35704.0
76.00	3088.0
76.80	329.0
78.10	222.0
78.90	2254.0
79.90	593.0
80.90	2485.0
81.80	447.0
86.90	1616.0
87.90	1500.0
90.80	344.0
91.90	2026.0
92.90	3024.0
94.00	7738.0
95.00	64176.0
96.00	4417.0
103.90	273.0
104.90	108.0
105.90	327.0
114.90	132.0
115.90	282.0
116.80	509.0
118.00	276.0
118.90	457.0
127.80	255.0
128.80	154.0
129.80	334.0
130.80	114.0
134.70	118.0
140.90	895.0
141.90	138.0
142.90	1147.0
144.80	170.0
147.80	208.0
150.00	103.0
154.90	100.0
156.80	146.0
160.90	107.0
171.80	502.0
173.90	52408.0
174.90	3472.0
175.90	49752.0
176.90	3205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.90	565.0
37.00	2543.0
38.00	2138.0
38.90	1045.0
39.80	127.0
44.00	284.0
44.90	406.0
46.90	319.0
48.00	433.0
49.00	2534.0
50.00	10719.0
51.00	3032.0
51.90	137.0
55.00	142.0
56.00	843.0
57.00	1653.0
59.90	803.0
61.00	3382.0
62.00	3184.0
63.00	2556.0
63.90	319.0
65.00	615.0
68.00	6824.0
69.00	6382.0
69.90	350.0
71.00	404.0
73.90	3566.0
74.00	12571.0
75.00	36752.0
76.00	3081.0
76.80	313.0
78.10	215.0
78.90	2218.0
79.90	568.0
80.90	2525.0
81.80	429.0
86.90	1908.0
87.90	1680.0
90.80	347.0
91.90	1996.0
93.00	3208.0
94.00	7811.0
95.00	65944.0
96.00	4281.0
96.90	119.0
103.80	284.0
104.90	108.0
105.90	342.0
114.90	104.0
115.70	239.0
116.80	581.0
117.90	313.0
118.90	465.0
127.80	256.0
128.80	151.0
129.80	394.0
134.80	110.0
136.80	100.0
140.90	972.0
141.80	180.0
142.90	1169.0
144.90	159.0
147.80	206.0
154.80	128.0
156.80	151.0
160.80	105.0
171.80	477.0
173.90	55504.0
174.90	3642.0
175.90	52544.0
176.90	3201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.90	556.0
36.90	2284.0
37.90	2070.0
38.90	980.0
39.80	104.0
43.80	245.0
44.90	378.0
46.90	304.0
47.90	406.0
49.00	2376.0
50.00	10106.0
51.00	2663.0
51.90	174.0
55.10	125.0
56.00	782.0
57.00	1535.0
60.00	778.0
61.00	3028.0
62.00	2852.0
63.00	2333.0
63.90	271.0
65.00	564.0
67.10	137.0
68.00	6522.0
69.00	6084.0
69.90	297.0
71.90	387.0
73.00	3200.0
74.00	11696.0
75.00	34704.0
76.00	2820.0
76.80	276.0
78.10	191.0
78.90	1927.0
79.90	486.0
80.90	2226.0
81.80	430.0
86.90	1942.0
87.90	1733.0
90.90	314.0
92.00	1880.0
92.90	3004.0
94.00	7314.0
95.00	61368.0
96.00	3833.0
97.00	121.0
103.80	289.0
104.90	103.0
105.90	320.0
115.70	233.0
116.00	240.0
116.80	573.0
117.80	328.0
118.90	437.0
127.80	243.0
128.80	124.0
129.80	400.0
134.90	141.0
136.80	122.0
140.90	1008.0
141.80	192.0
142.90	1076.0
144.80	180.0
147.70	189.0
154.70	165.0
156.80	127.0
171.80	419.0
173.90	52944.0
174.90	3567.0
175.90	50552.0
176.90	2888.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063