


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU011819\
Data File : VU029213.D
Acq On : 18 Jan 2019 08:29
Operator : JC/SP
Sample : BFB71
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB71

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jan 18 23:01:06 2019

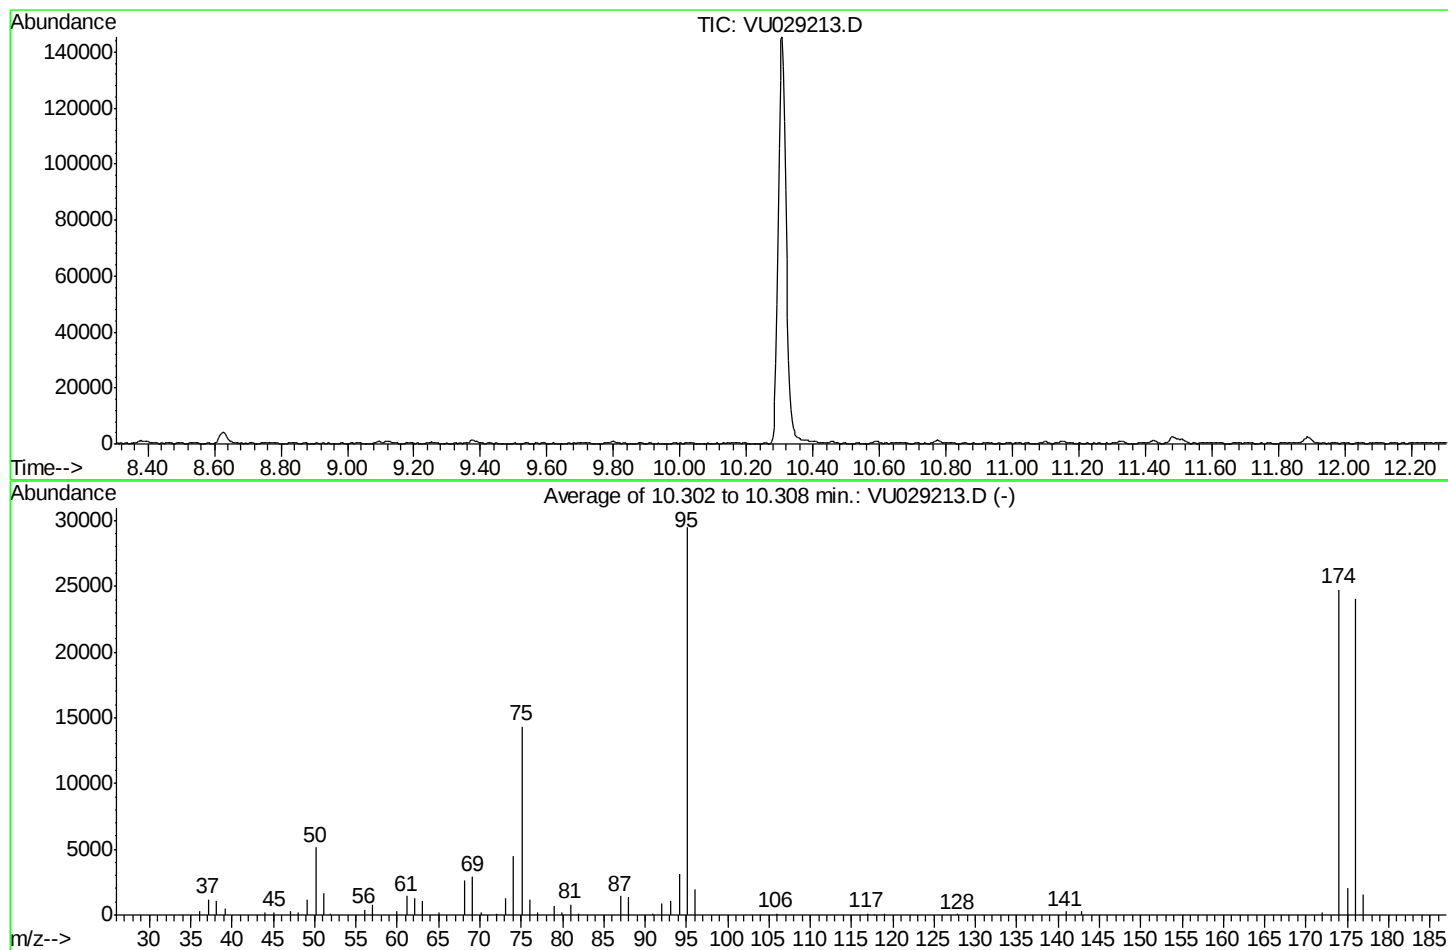

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	5136	PASS
75	95	30	80	48.6	14318	PASS
95	95	100	100	100.0	29485	PASS
96	95	5	9	6.7	1967	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	24760	PASS
175	174	5	9	8.1	2014	PASS
176	174	95	101	97.1	24050	PASS
177	176	5	9	6.4	1547	PASS

m/z	Abundance
44.00	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB71

m/z	Abundance
36.00	246.0
37.10	1123.0
38.10	1044.0
39.10	435.0
44.00	317.0
45.10	158.0
47.00	295.0
48.00	150.0
49.10	1096.0
50.10	4911.0
51.10	1516.0
51.90	101.0
56.00	388.0
57.00	695.0
60.00	278.0
61.10	1435.0
62.10	1227.0
63.10	1005.0
65.00	199.0
68.10	2448.0
69.10	2727.0
70.10	206.0
72.10	170.0
73.10	1162.0
74.10	4132.0
75.10	13317.0
76.10	1147.0
76.90	135.0
79.00	701.0
79.90	188.0
81.00	738.0
81.90	128.0
87.00	1338.0
88.00	1313.0
92.10	822.0
93.10	1043.0
94.10	2813.0
95.10	28152.0
96.00	1888.0
105.90	120.0
117.00	134.0
127.90	102.0
140.90	295.0
142.90	250.0
171.90	230.0
174.00	22608.0
175.00	1830.0
176.00	21648.0
177.00	1480.0

Instrument :
MSVOA_U
ClientSampleId :
BFB71

m/z	Abundance
36.00	277.0
37.10	1245.0
38.10	1136.0
39.10	482.0
44.00	370.0
45.10	213.0
47.10	314.0
48.00	172.0
49.10	1163.0
50.10	5273.0
51.10	1719.0
51.90	120.0
56.00	449.0
57.00	778.0
60.00	270.0
61.10	1499.0
62.10	1327.0
63.10	1090.0
65.00	218.0
68.10	2725.0
69.10	2976.0
70.10	231.0
72.00	130.0
73.10	1316.0
74.10	4653.0
75.10	14741.0
76.00	1213.0
77.00	141.0
78.90	735.0
79.90	221.0
81.00	836.0
81.90	134.0
87.00	1507.0
88.00	1369.0
91.00	133.0
92.00	947.0
93.00	1150.0
94.10	3247.0
95.10	30376.0
96.10	2018.0
105.90	136.0
116.90	136.0
119.00	130.0
127.80	100.0
140.90	307.0
142.90	290.0
171.90	240.0
174.00	25512.0
175.00	2070.0
176.00	24808.0
177.00	1618.0

Instrument :
MSVOA_U
ClientSampleId :
BFB71

m/z	Abundance
36.00	273.0
37.10	1284.0
38.10	1168.0
39.10	445.0
44.00	399.0
45.10	253.0
47.10	320.0
48.00	192.0
49.10	1115.0
50.10	5224.0
51.10	1729.0
56.00	459.0
57.00	763.0
60.00	234.0
61.10	1325.0
62.10	1365.0
63.00	1036.0
65.10	224.0
68.10	2735.0
69.10	2982.0
70.10	220.0
71.90	129.0
73.10	1355.0
74.10	4651.0
75.10	14896.0
76.00	1192.0
77.00	180.0
78.90	701.0
79.90	234.0
81.00	837.0
82.00	123.0
87.00	1462.0
88.00	1294.0
90.90	144.0
92.00	953.0
93.00	1130.0
94.10	3436.0
95.10	29928.0
96.10	1996.0
104.00	108.0
105.90	123.0
116.90	154.0
117.80	104.0
119.00	153.0
140.90	271.0
142.90	304.0
171.90	236.0
174.00	26160.0
175.00	2142.0
176.00	25696.0
177.00	1543.0

Instrument :
MSVOA_U
ClientSampleId :
BFB71