

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
 Data File : VU042089.D
 Acq On : 18 Jan 2021 12:27
 Operator : SY/MD
 Sample : VU0118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
 Title : VOC Analysis

Signal : TIC: VU042089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	91	rVB	178186	189115	16.60%	2.432%
2	1.919	171	180	192	rBV	137704	173525	15.23%	2.231%
3	2.469	349	351	355	rBV	312	224	0.02%	0.003%
4	2.578	372	385	415	rBV	248768	413893	36.33%	5.322%
5	2.736	430	434	436	rBV2	365	274	0.02%	0.004%
6	2.803	447	455	468	rBV3	1174	2343	0.21%	0.030%
7	2.986	509	512	517	rBV2	358	395	0.03%	0.005%
8	3.054	527	533	546	rBB3	1139	1515	0.13%	0.019%
9	3.157	563	565	569	rBV	154	104	0.01%	0.001%
10	3.372	629	632	637	rBV2	454	433	0.04%	0.006%
11	3.401	638	641	645	rVV2	266	200	0.02%	0.003%
12	3.597	695	702	704	rBV	209	296	0.03%	0.004%
13	3.697	730	733	734	rBV	184	126	0.01%	0.002%
14	3.768	752	755	759	rBV	186	118	0.01%	0.002%
15	3.986	820	823	826	rVB2	306	218	0.02%	0.003%
16	4.006	827	829	831	rBV	291	180	0.02%	0.002%
17	4.105	857	860	864	rBV2	219	189	0.02%	0.002%
18	4.350	934	936	938	rBV	150	102	0.01%	0.001%
19	4.375	941	944	945	rBV	174	102	0.01%	0.001%
20	4.459	967	970	972	rBV	197	152	0.01%	0.002%
21	4.475	972	975	981	rVV2	228	211	0.02%	0.003%
22	4.517	985	988	991	rBV	187	191	0.02%	0.002%
23	4.581	1003	1008	1012	rBV2	354	467	0.04%	0.006%
24	4.645	1012	1028	1060	rBV	108719	285421	25.06%	3.670%
25	4.948	1120	1122	1123	rBV	243	105	0.01%	0.001%
26	5.015	1141	1143	1146	rBV	204	110	0.01%	0.001%
27	5.080	1146	1163	1185	rBV	205265	450158	39.52%	5.788%
28	5.250	1214	1216	1218	rBV	231	130	0.01%	0.002%
29	5.266	1218	1221	1223	rVB2	291	140	0.01%	0.002%
30	5.305	1226	1233	1238	rBV3	899	1179	0.10%	0.015%
31	5.385	1255	1258	1260	rBV	297	231	0.02%	0.003%
32	5.501	1291	1294	1296	rBB	218	130	0.01%	0.002%
33	5.520	1299	1300	1302	rBV	128	71	0.01%	0.001%
34	5.533	1302	1304	1308	rVB3	236	148	0.01%	0.002%
35	5.636	1333	1336	1337	rBV	147	102	0.01%	0.001%
36	5.739	1346	1368	1396	rBV2	426337	1139168	100.00%	14.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
 Data File : VU042089.D
 Acq On : 18 Jan 2021 12:27
 Operator : SY/MD
 Sample : VU0118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
 Title : VOC Analysis

37	6.044	1460	1463	1466	rBV	355	267	0.02%	0.003%
38	6.176	1499	1504	1507	rBV2	277	238	0.02%	0.003%
39	6.195	1507	1510	1515	rVB	223	118	0.01%	0.002%
40	6.263	1515	1531	1550	rBV	324759	616752	54.14%	7.930%
41	6.510	1606	1608	1610	rBV	286	132	0.01%	0.002%
42	6.542	1610	1618	1628	rVB5	2973	4827	0.42%	0.062%
43	6.610	1636	1639	1643	rBV2	337	319	0.03%	0.004%
44	6.700	1653	1667	1692	rBV	235618	458138	40.22%	5.891%
45	6.816	1699	1703	1709	rVB2	491	531	0.05%	0.007%
46	6.893	1725	1727	1730	rBV	151	71	0.01%	0.001%
47	6.951	1743	1745	1748	rBB	177	119	0.01%	0.002%
48	6.973	1749	1752	1755	rBB	224	111	0.01%	0.001%
49	7.047	1773	1775	1776	rBV	143	77	0.01%	0.001%
50	7.121	1795	1798	1799	rBV	229	114	0.01%	0.001%
51	7.157	1806	1809	1811	rBB	176	115	0.01%	0.001%
52	7.176	1812	1815	1819	rBV	194	238	0.02%	0.003%
53	7.250	1832	1838	1842	rBV	184	307	0.03%	0.004%
54	7.285	1846	1849	1853	rVV	142	96	0.01%	0.001%
55	7.350	1866	1869	1872	rBV	171	168	0.01%	0.002%
56	7.420	1889	1891	1896	rBV	189	209	0.02%	0.003%
57	7.575	1923	1939	1961	rBV	122680	216169	18.98%	2.779%
58	7.700	1976	1978	1979	rBV	243	96	0.01%	0.001%
59	7.726	1983	1986	1993	rVB	342	327	0.03%	0.004%
60	7.758	1994	1996	1999	rBB	188	118	0.01%	0.002%
61	7.774	1999	2001	2003	rBV2	253	142	0.01%	0.002%
62	7.793	2003	2007	2008	rBV2	885	659	0.06%	0.008%
63	7.906	2028	2042	2063	rBV	436595	759482	66.67%	9.765%
64	8.185	2117	2129	2147	rBV	90027	151408	13.29%	1.947%
65	8.404	2195	2197	2203	rBV	212	223	0.02%	0.003%
66	8.475	2216	2219	2224	rBV2	268	290	0.03%	0.004%
67	8.562	2243	2246	2249	rBB	292	224	0.02%	0.003%
68	8.591	2250	2255	2258	rBB	157	149	0.01%	0.002%
69	8.639	2258	2270	2303	rBV	273421	514998	45.21%	6.622%
70	8.983	2374	2377	2381	rBV2	236	156	0.01%	0.002%
71	9.079	2404	2407	2410	rBV	194	191	0.02%	0.002%
72	9.195	2436	2443	2445	rBV	204	269	0.02%	0.003%
73	9.243	2455	2458	2460	rVB	187	100	0.01%	0.001%
74	9.304	2473	2477	2479	rBV	178	159	0.01%	0.002%
75	9.420	2500	2513	2549	rVB	386983	648881	56.96%	8.343%
76	9.565	2550	2558	2562	rBV3	669	841	0.07%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
 Data File : VU042089.D
 Acq On : 18 Jan 2021 12:27
 Operator : SY/MD
 Sample : VU0118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M

Title : VOC Analysis

77	9.639	2577	2581	2588	rBV2	373	416	0.04%	0.005%
78	9.693	2596	2598	2604	rVB2	576	408	0.04%	0.005%
79	9.735	2609	2611	2614	rBV2	182	108	0.01%	0.001%
80	9.819	2634	2637	2639	rBV2	203	126	0.01%	0.002%
81	9.964	2680	2682	2686	rBV	316	285	0.03%	0.004%
82	10.250	2768	2771	2774	rBV	128	84	0.01%	0.001%
83	10.510	2849	2852	2854	rBV	523	419	0.04%	0.005%
84	10.629	2884	2889	2900	rVB6	1017	1736	0.15%	0.022%
85	10.755	2916	2928	2948	rVB	293905	477565	41.92%	6.140%
86	10.899	2971	2973	2981	rVB	182	144	0.01%	0.002%
87	11.086	3026	3031	3035	rBV3	545	563	0.05%	0.007%
88	11.465	3144	3149	3154	rBV3	597	686	0.06%	0.009%
89	11.639	3200	3203	3204	rBV	177	110	0.01%	0.001%
90	11.809	3243	3256	3272	rBV	377184	599184	52.60%	7.704%
91	12.189	3361	3374	3390	rBV	399755	648594	56.94%	8.339%
92	12.259	3394	3396	3399	rBV	328	222	0.02%	0.003%
93	12.481	3462	3465	3471	rVB	340	279	0.02%	0.004%
94	12.558	3485	3489	3493	rBV	237	249	0.02%	0.003%
95	13.214	3687	3693	3699	rVB2	1216	1562	0.14%	0.020%
96	13.356	3734	3737	3739	rBV2	273	185	0.02%	0.002%
97	13.452	3765	3767	3768	rBV	350	136	0.01%	0.002%
98	13.828	3878	3884	3894	rVB4	1882	2487	0.22%	0.032%
99	14.324	4030	4038	4044	rVB5	1798	2545	0.22%	0.033%
100	14.623	4129	4131	4132	rBV5	221	83	0.01%	0.001%




Sum of corrected areas: 7777471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
Data File : VU042089.D
Acq On : 18 Jan 2021 12:27
Operator : SY/MD
Sample : VU0118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

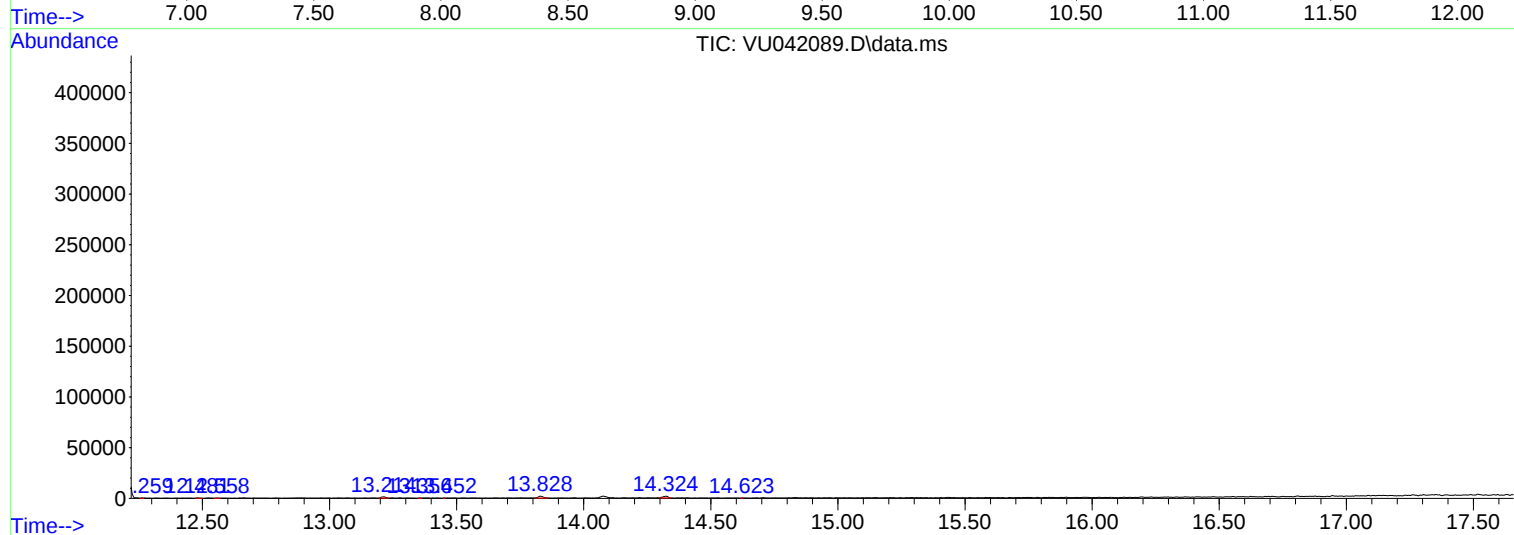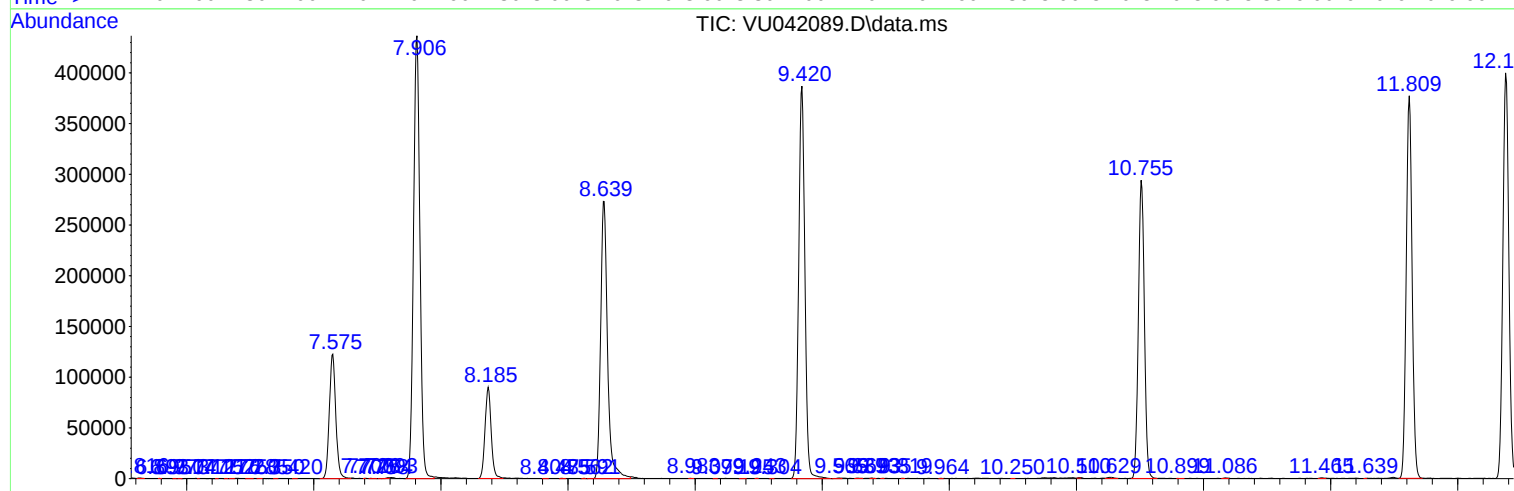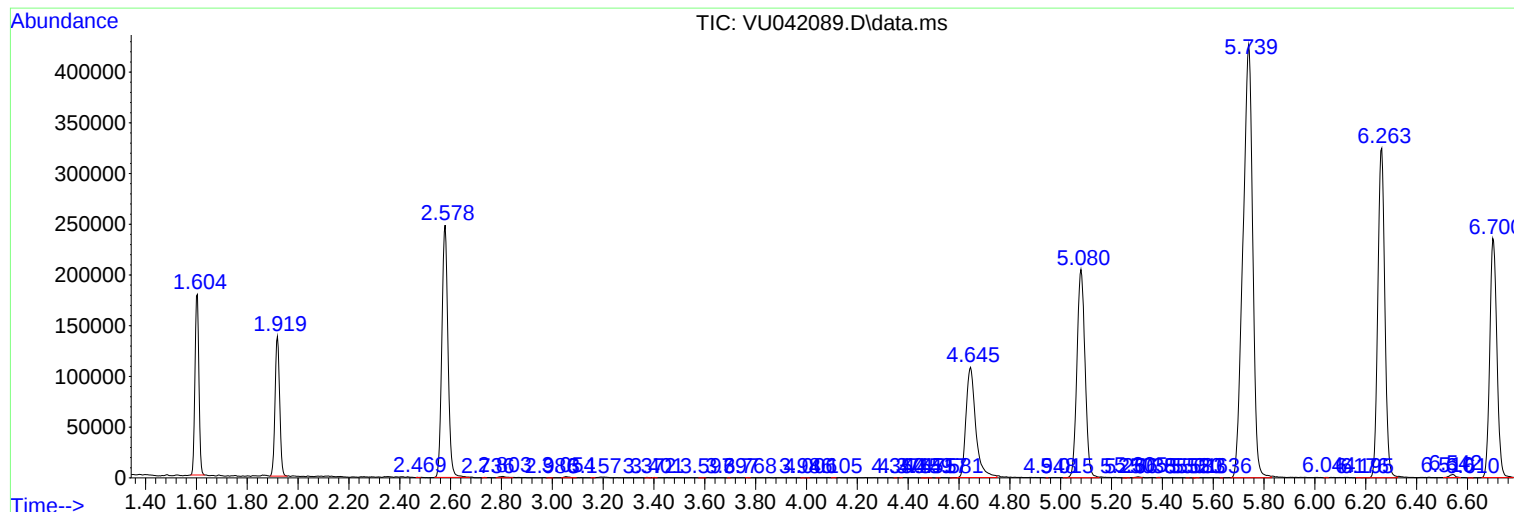

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
Data File : VU042089.D
Acq On : 18 Jan 2021 12:27
Operator : SY/MD
Sample : VU0118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
Data File : VU042089.D
Acq On : 18 Jan 2021 12:27
Operator : SY/MD
Sample : VU0118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
