
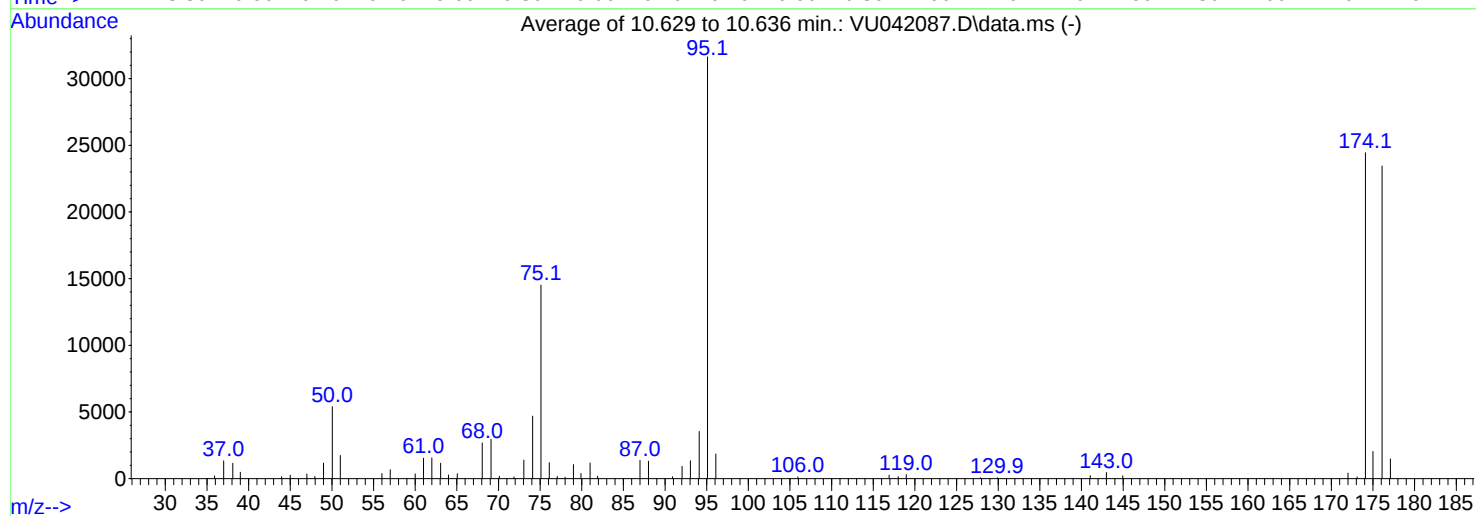


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011821\
 Data File : VU042087.D
 Acq On : 18 Jan 2021 10:16
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB603

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
 Title : VOC Analysis
 Last Update : Tue Jan 19 01:00:57 2021

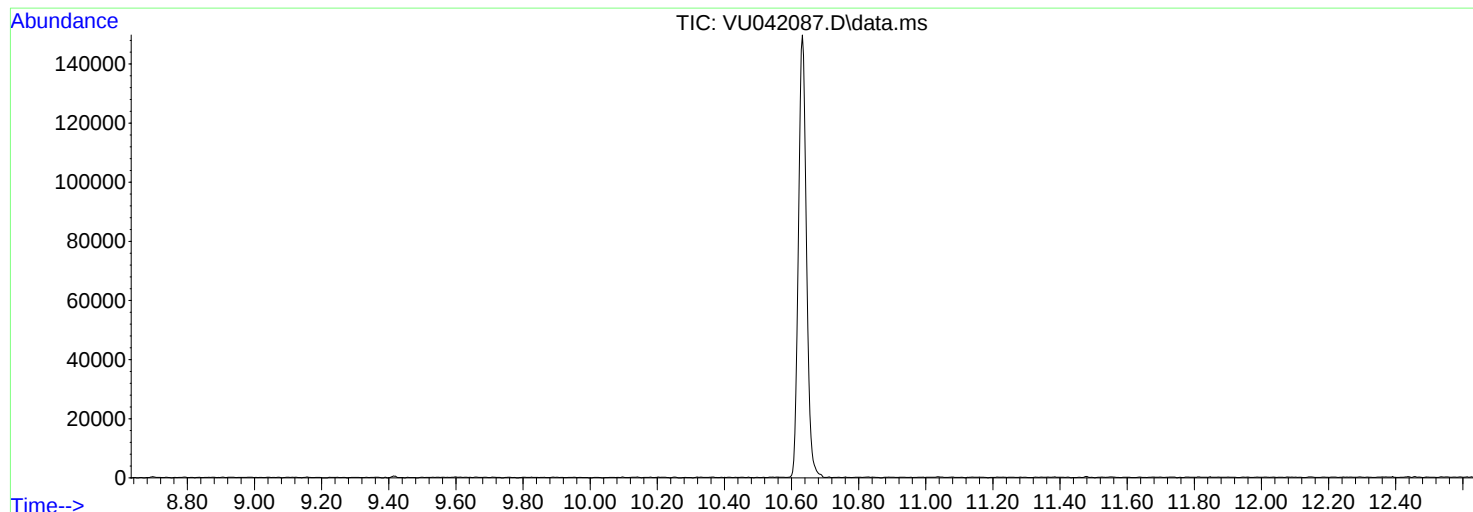

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5404	PASS
75	95	30	80	45.9	14520	PASS
95	95	100	100	100.0	31637	PASS
96	95	5	9	5.9	1854	PASS
173	174	0.00	2	0.5	131	PASS
174	95	50	120	77.3	24443	PASS
175	174	5	9	8.3	2037	PASS
176	174	95	101	95.9	23451	PASS
177	176	5	9	6.3	1475	PASS