


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011822\
 Data File : VU046772.D
 Acq On : 18 Jan 2022 09:11
 Operator : SY/MD
 Sample : BFB044
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB044

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jan 20 02:00:32 2022

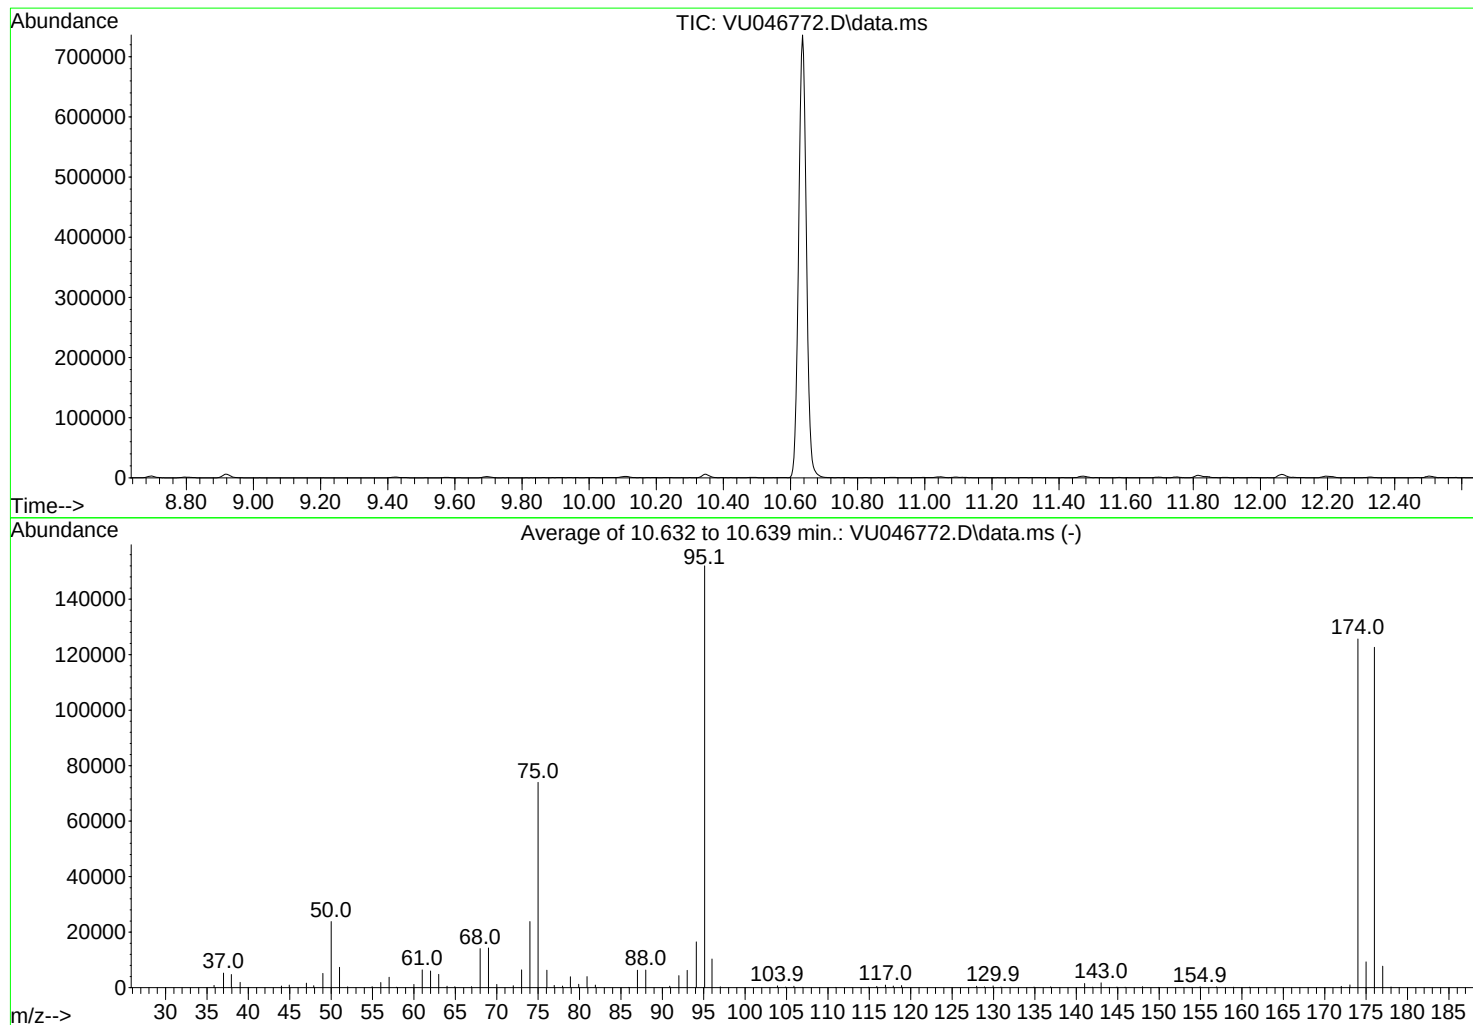

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	23795	PASS
75	95	30	80	48.7	73960	PASS
95	95	100	100	100.0	152000	PASS
96	95	5	9	6.8	10332	PASS
173	174	0.00	2	0.8	962	PASS
174	95	50	120	82.7	125653	PASS
175	174	5	9	7.4	9279	PASS
176	174	95	101	97.6	122643	PASS
177	176	5	9	6.3	7714	PASS

m/z	Abundance
35.90	237.0
37.80	106.0
44.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	1056.0
37.00	5487.0
38.00	4981.0
39.00	1941.0
40.00	137.0
44.00	710.0
45.00	971.0
47.00	1698.0
47.90	694.0
49.00	5271.0
50.00	24632.0
51.00	7575.0
52.00	319.0
55.00	370.0
56.00	1893.0
57.00	3912.0
57.90	168.0
60.00	1182.0
61.00	6626.0
62.00	6131.0
63.00	4885.0
64.00	508.0
65.00	345.0
66.90	346.0
68.00	14569.0
69.00	14776.0
70.00	1163.0
72.00	743.0
73.00	6565.0
74.00	24568.0
75.00	76256.0
76.00	6508.0
77.00	811.0
77.90	603.0
78.90	4100.0
79.90	1237.0
80.90	4134.0
81.90	943.0
85.90	140.0
87.00	6428.0
88.00	6464.0
90.90	543.0
92.00	4468.0
93.00	6479.0
94.10	16920.0
95.10	156864.0
96.00	10700.0
97.00	310.0
103.90	680.0
104.90	254.0
105.90	525.0
106.90	132.0
111.00	115.0
112.90	116.0
114.90	174.0
115.90	510.0
116.90	963.0
117.90	560.0
118.90	780.0
127.90	548.0
128.90	270.0
129.90	641.0
130.90	228.0
134.90	252.0
136.90	292.0
141.00	1612.0
142.00	180.0
143.00	1771.0
143.90	136.0
144.90	214.0
145.90	177.0
148.00	362.0
149.90	138.0
153.00	114.0
155.00	381.0
156.90	276.0
159.00	198.0
160.90	196.0
172.00	456.0
173.10	976.0
174.00	129304.0
175.00	9598.0
176.00	126688.0
177.00	7961.0
178.00	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	899.0
37.00	5023.0
38.00	4636.0
39.00	1777.0
40.00	116.0
44.00	643.0
44.90	919.0
47.00	1561.0
47.90	633.0
49.00	4884.0
50.00	23096.0
51.00	7325.0
52.00	303.0
54.90	331.0
56.00	1845.0
57.00	3467.0
57.90	166.0
60.00	1048.0
61.00	6219.0
62.00	5836.0
63.00	4706.0
64.00	464.0
65.00	287.0
66.90	330.0
68.00	13642.0
69.00	13893.0
70.00	1081.0
72.00	689.0
73.00	6266.0
74.00	23128.0
75.00	72672.0
76.00	5925.0
76.90	707.0
77.90	562.0
78.90	3849.0
79.90	1140.0
80.90	3769.0
81.90	887.0
86.00	136.0
87.00	6324.0
88.00	6214.0
90.90	481.0
92.00	4297.0
93.00	5994.0
94.10	16327.0
95.10	148864.0
96.00	9947.0
97.00	245.0
103.90	675.0
104.90	273.0
105.90	563.0
106.90	116.0
111.00	117.0
114.90	182.0
115.90	481.0
117.00	899.0
117.90	544.0
118.90	739.0
127.90	501.0
128.90	293.0
130.00	618.0
130.90	240.0
134.90	222.0
136.90	265.0
141.00	1409.0
142.00	159.0
143.00	1686.0
143.90	136.0
144.90	215.0
145.90	166.0
148.00	377.0
150.00	142.0
152.90	129.0
154.90	332.0
156.90	260.0
159.00	148.0
160.90	175.0
172.00	417.0
173.10	971.0
174.00	126592.0
175.00	9121.0
176.00	123232.0
177.00	7732.0
178.00	229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.00	1134.0
37.00	5298.0
38.00	4838.0
39.00	1932.0
40.00	150.0
44.00	771.0
44.90	937.0
47.00	1631.0
47.90	727.0
49.00	5186.0
50.00	23656.0
51.00	7100.0
52.00	326.0
55.00	390.0
56.00	1888.0
57.00	3883.0
57.90	156.0
60.00	1258.0
61.00	6335.0
62.00	6086.0
63.00	4737.0
64.00	535.0
64.90	419.0
67.00	355.0
68.00	13968.0
69.00	14171.0
70.00	1149.0
72.00	732.0
73.00	6314.0
74.00	23752.0
75.00	72952.0
76.10	6511.0
77.00	837.0
78.00	596.0
78.90	3874.0
79.90	1221.0
80.90	4011.0
81.90	881.0
85.90	127.0
87.00	6096.0
88.00	6285.0
90.90	495.0
92.00	4262.0
93.00	6317.0
94.10	16148.0
95.10	150272.0
96.00	10348.0
97.00	342.0
103.90	605.0
104.90	191.0
105.90	513.0
107.00	128.0
110.90	108.0
112.90	114.0
114.90	169.0
115.90	495.0
117.00	931.0
117.90	553.0
118.90	753.0
128.00	571.0
128.90	257.0
129.90	606.0
130.90	219.0
134.90	238.0
136.90	267.0
141.00	1565.0
141.90	169.0
143.00	1665.0
144.00	119.0
144.90	208.0
145.90	195.0
148.00	316.0
149.90	143.0
153.90	101.0
155.00	424.0
157.00	256.0
159.00	218.0
160.90	172.0
172.00	485.0
173.00	939.0
174.00	121064.0
175.00	9119.0
176.00	118008.0
177.00	7448.0
178.00	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044