
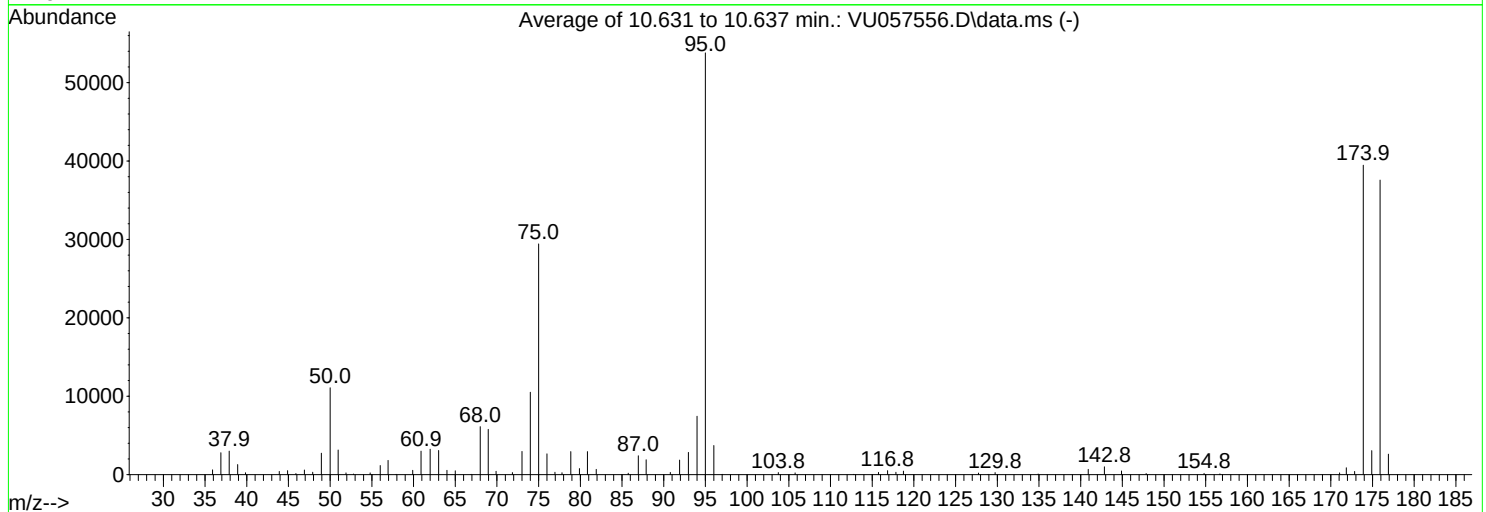


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011824\
Data File : VU057556.D
Acq On : 18 Jan 2024 13:00
Operator : MD/SY
Sample : BFB034
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB034

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011824WMA.M
Title : VOC Analysis
Last Update : Fri Jan 19 01:50:34 2024

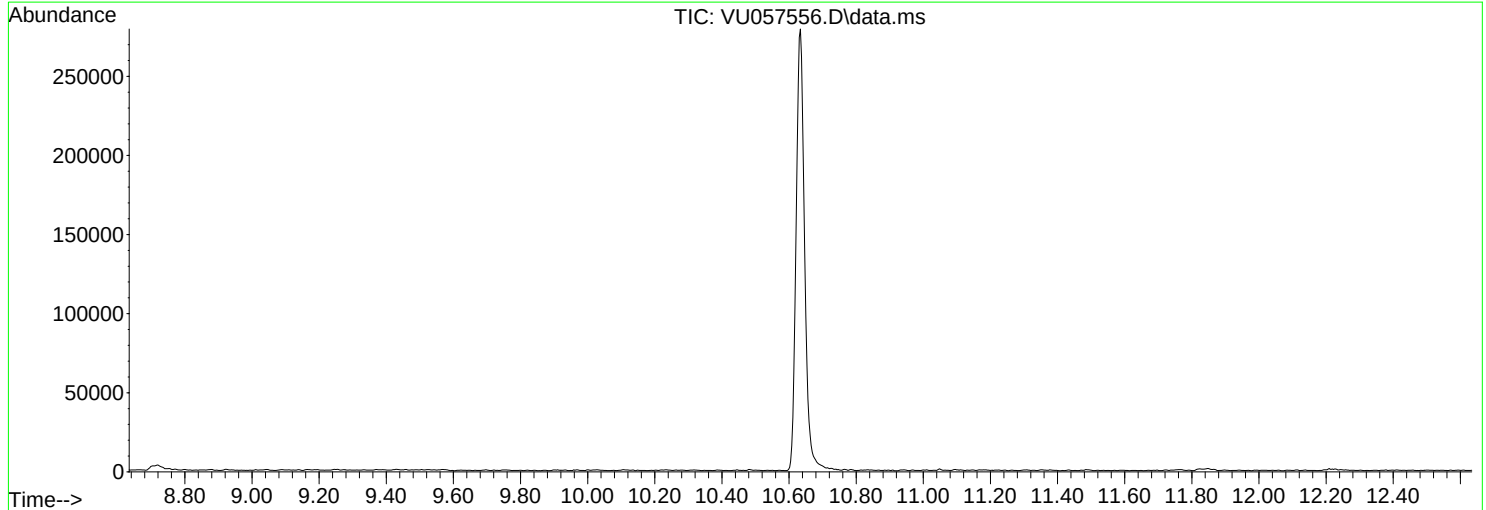

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	11082	PASS
75	95	30	80	54.7	29427	PASS
95	95	100	100	100.0	53800	PASS
96	95	5	9	6.9	3716	PASS
173	174	0.00	2	1.0	412	PASS
174	95	50	120	73.4	39477	PASS
175	174	5	9	7.8	3070	PASS
176	174	95	101	95.2	37565	PASS
177	176	5	9	7.0	2619	PASS

m/z	Abundance
39.80	386.0
43.90	420.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	682.0
36.90	2797.0
37.90	2935.0
38.90	1414.0
40.00	614.0
43.90	724.0
44.90	558.0
45.90	143.0
46.90	734.0
47.90	329.0
49.00	2915.0
50.00	10962.0
50.90	3282.0
51.90	214.0
54.80	270.0
56.00	1237.0
56.90	2031.0
57.90	139.0
59.90	539.0
60.90	2822.0
62.00	3264.0
63.00	2999.0
64.00	542.0
65.00	488.0
66.90	109.0
68.00	6144.0
68.90	5989.0
69.80	388.0
71.80	308.0
73.00	2928.0
74.00	10411.0
75.00	29624.0
76.00	2897.0
77.00	394.0
77.80	306.0
78.90	3085.0
79.90	769.0
80.90	2831.0
81.90	684.0
85.80	138.0
86.90	2348.0
87.90	1689.0
90.80	340.0
91.90	1738.0
93.00	2726.0
94.00	7659.0
95.00	54336.0
96.00	3954.0
103.70	251.0
105.70	270.0
112.80	100.0
115.80	303.0
116.80	488.0
117.80	327.0
118.70	471.0
127.70	192.0
128.90	114.0
129.80	197.0
134.90	140.0
140.90	752.0
142.80	908.0
144.90	437.0
147.90	151.0
154.80	179.0
156.70	105.0
171.00	251.0
171.90	930.0
172.80	350.0
173.90	39688.0
174.90	3043.0
175.90	37536.0
176.90	2952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	622.0
36.90	2903.0
37.90	3094.0
38.90	1350.0
40.00	619.0
43.90	883.0
44.90	521.0
45.90	164.0
46.90	609.0
47.90	326.0
48.90	2809.0
50.00	11355.0
51.00	3304.0
51.90	238.0
52.80	121.0
54.80	232.0
56.00	1198.0
56.90	1852.0
59.90	552.0
60.90	3084.0
62.00	3343.0
63.00	3132.0
64.00	580.0
65.00	490.0
68.00	6373.0
69.00	5892.0
69.90	433.0
71.80	267.0
73.00	3096.0
74.00	10734.0
75.00	30552.0
76.00	2706.0
76.90	278.0
77.80	256.0
78.80	3008.0
79.90	802.0
80.90	2968.0
81.90	682.0
85.70	208.0
86.90	2464.0
87.90	1923.0
90.80	300.0
91.90	1911.0
93.00	2909.0
94.00	7651.0
95.00	55472.0
96.00	3807.0
103.80	269.0
105.70	244.0
115.80	298.0
116.80	539.0
117.90	292.0
118.70	432.0
127.80	204.0
129.70	263.0
134.90	131.0
140.90	685.0
142.90	1006.0
144.90	483.0
147.90	162.0
154.80	182.0
156.70	106.0
171.00	238.0
171.90	957.0
172.90	412.0
173.90	40584.0
174.90	3188.0
175.90	38480.0
176.90	2672.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	509.0
36.90	2719.0
37.90	2949.0
38.90	1122.0
39.90	633.0
43.90	879.0
44.90	463.0
45.90	128.0
46.90	462.0
47.90	290.0
48.90	2499.0
50.00	10929.0
51.00	2835.0
51.90	248.0
52.80	114.0
54.80	178.0
56.00	1081.0
57.00	1585.0
59.90	575.0
60.90	3116.0
62.00	3136.0
63.00	3109.0
64.00	546.0
65.00	496.0
68.00	5876.0
69.00	5427.0
70.00	458.0
71.90	216.0
73.00	2846.0
74.00	10411.0
75.00	28104.0
76.00	2356.0
76.90	240.0
77.90	184.0
78.80	2755.0
79.90	779.0
80.80	3018.0
81.90	677.0
85.70	195.0
87.00	2397.0
87.90	2090.0
90.80	239.0
91.90	1913.0
92.90	2877.0
94.00	7018.0
95.00	51592.0
96.00	3386.0
97.00	129.0
103.80	247.0
105.80	190.0
115.70	239.0
116.90	521.0
117.90	280.0
118.80	427.0
127.70	198.0
129.70	326.0
140.90	564.0
142.90	1063.0
144.90	472.0
147.80	138.0
154.80	149.0
156.70	106.0
171.10	201.0
171.80	769.0
172.90	474.0
173.90	38160.0
174.90	2980.0
175.90	36680.0
176.90	2234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034