


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011923\
Data File : VU052733.D
Acq On : 19 Jan 2023 12:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U011923W.M
Title : SW846 8260
Last Update : Fri Jan 20 01:04:16 2023

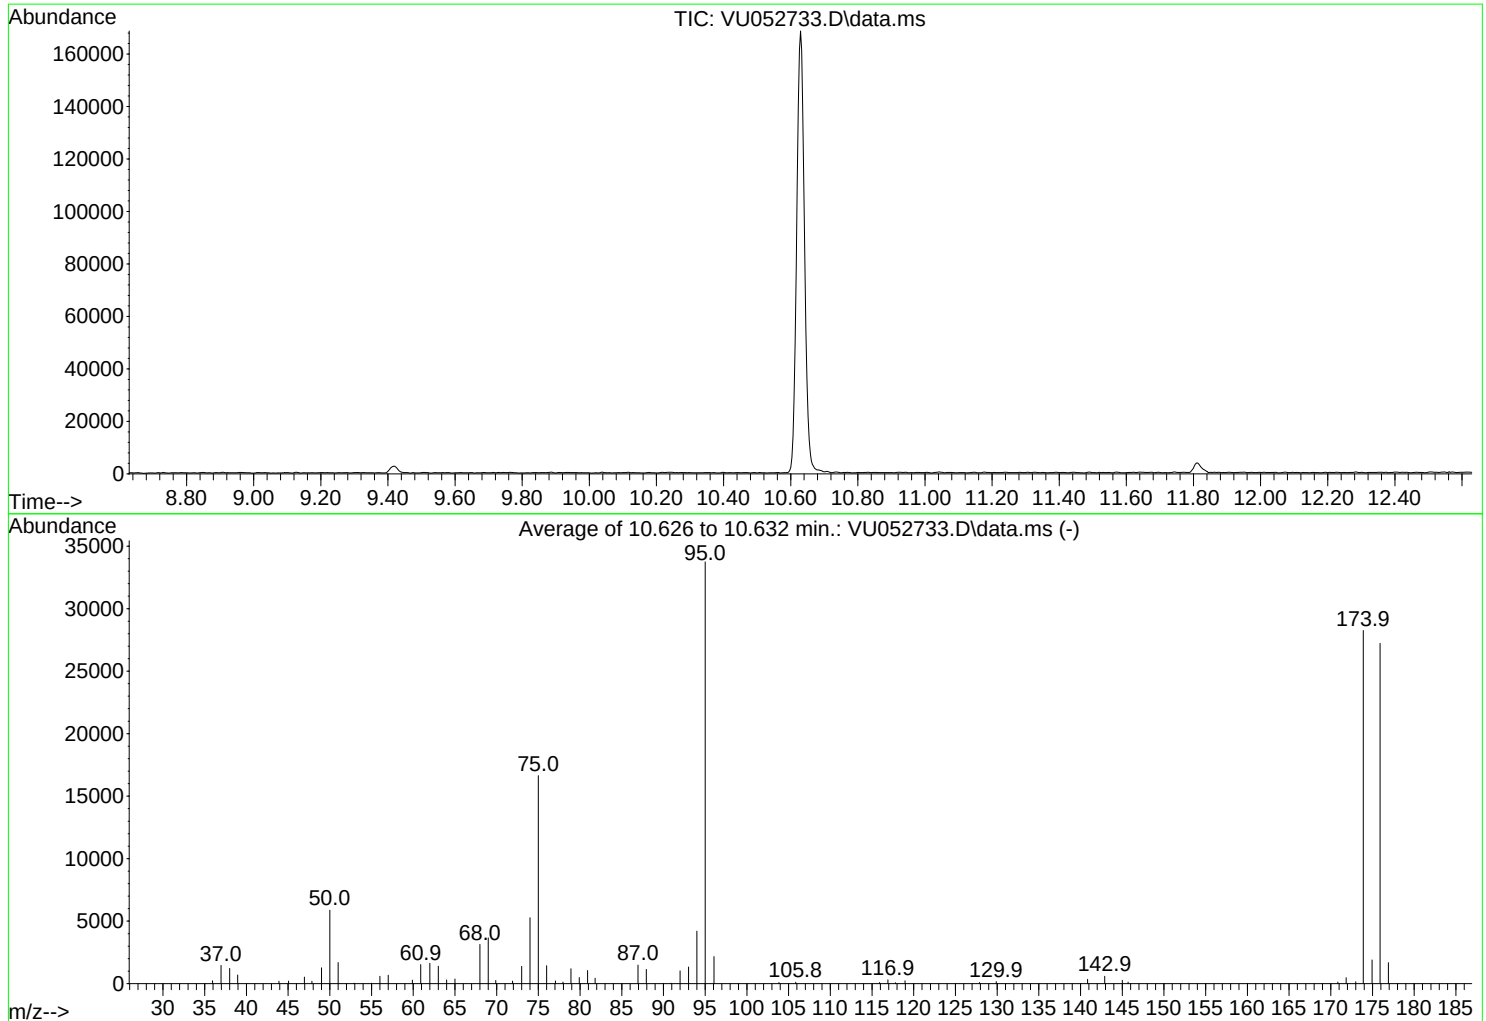

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	5879	PASS
75	95	30	60	49.3	16642	PASS
95	95	100	100	100.0	33747	PASS
96	95	5	9	6.4	2161	PASS
173	174	0.00	2	0.5	151	PASS
174	95	50	100	83.7	28259	PASS
175	174	5	9	6.7	1900	PASS
176	174	95	101	96.3	27224	PASS
177	176	5	9	6.2	1682	PASS