

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
 Data File : VU042105.D
 Acq On : 20 Jan 2021 14:59
 Operator : SY/MD
 Sample : VIBLK01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK01

Quant Time: Jan 21 04:21:56 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jan 21 04:09:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	120060	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	112796	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	58651	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	38069	4.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.20%
7) Chloroethane-d5	1.916	69	30618	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.571	63	62670	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	4.652	46	167062	59.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.24%
24) Chloroform-d	5.073	84	78233	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.713	65	49878	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.735	84	146209	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.700	67	49118	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.906	98	137636	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
43) trans-1,3-Dichloroprop...	8.189	79	25040	5.20	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.00%
46) 2-Hexanone-d5	8.645	63	123213	58.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.52%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	43843	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	55326	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%
Target Compounds						
16) Methylene chloride	3.054	84	6702	0.70	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042105.D
Acq On : 20 Jan 2021 14:59
Operator : SY/MD
Sample : VIBLK01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK01


Quant Time: Jan 21 04:21:56 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jan 21 04:09:50 2021
Response via : Initial Calibration

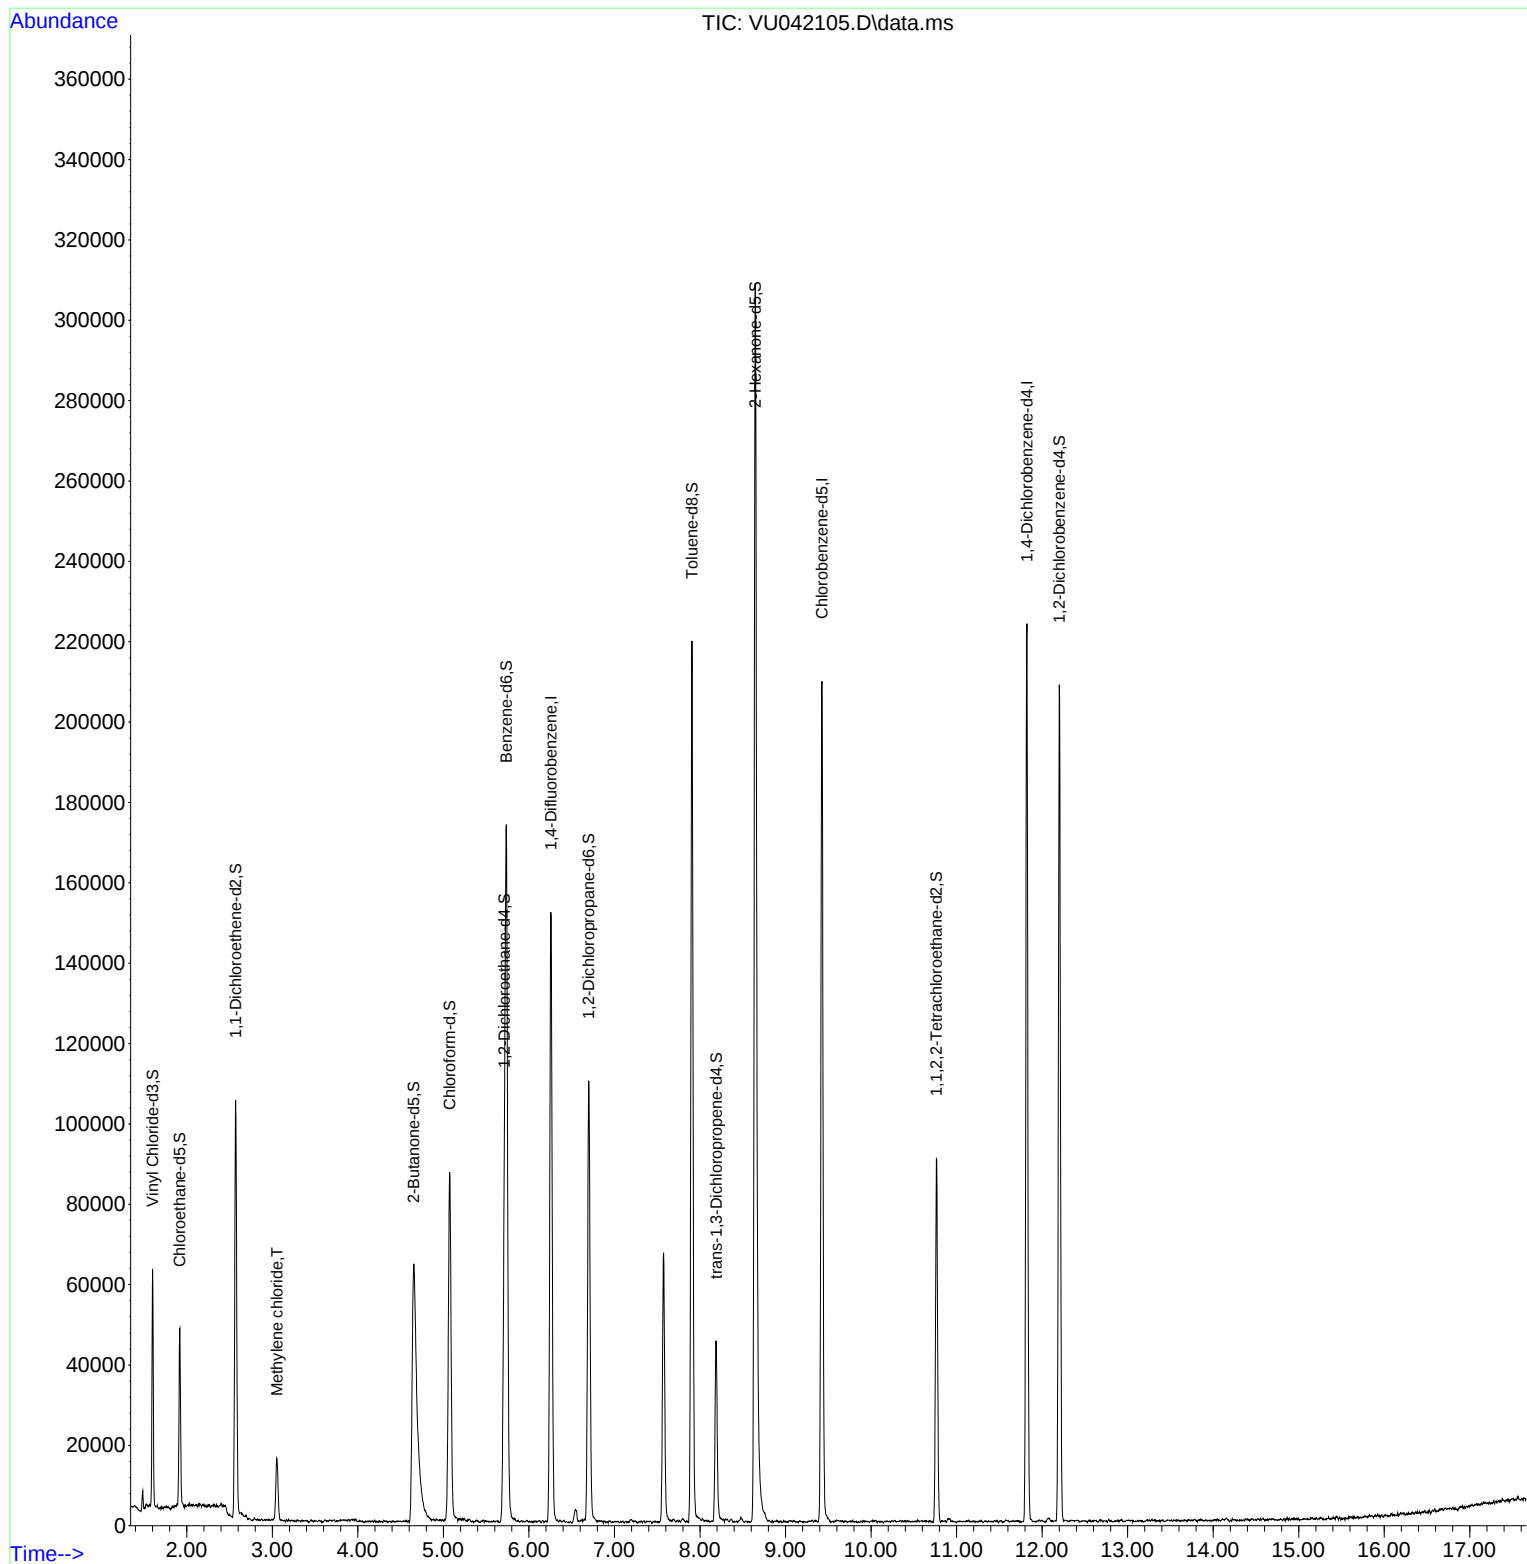

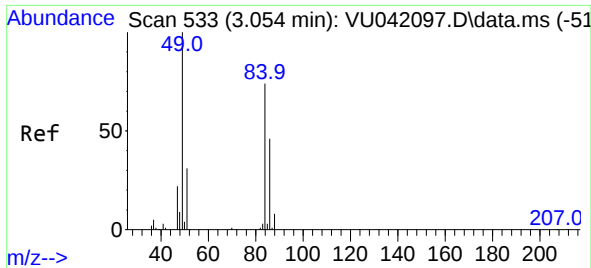

#16
Methylene chloride
Concen: 0.70 ug/L
RT: 3.054 min Scan# 533
Delta R.T. 0.000 min
Lab File: VU042105.D
Acq: 20 Jan 2021 14:59

Instrument :
MSVOA_U
ClientSampleId :
VIBLK01

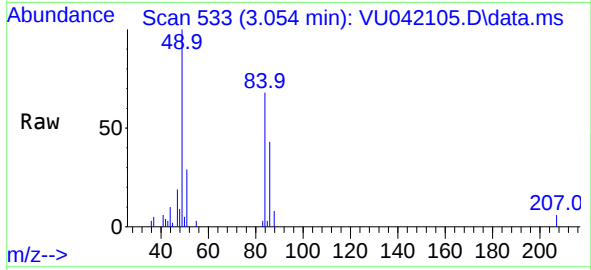

Tgt Ion: 84 Resp: 6702

Ion	Ratio	Lower	Upper
84	100		
86	62.8	44.1	81.9
49	147.3	95.0	176.4

