

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
 Data File : VU042121.D
 Acq On : 20 Jan 2021 21:57
 Operator : SY/MD
 Sample : VU0120WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK22

Quant Time: Jan 21 06:01:45 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jan 21 06:00:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	114253	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	104453	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	53633	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	38707	5.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.00%
7) Chloroethane-d5	1.919	69	31701	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%
11) 1,1-Dichloroethene-d2	2.572	63	64146	3.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.00%
20) 2-Butanone-d5	4.649	46	154447	57.43	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.86%
24) Chloroform-d	5.073	84	81008	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.20%
26) 1,2-Dichloroethane-d4	5.713	65	49649	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.80%
32) Benzene-d6	5.736	84	152492	5.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.80%
36) 1,2-Dichloropropane-d6	6.700	67	49479	5.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.40%
41) Toluene-d8	7.906	98	139247	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.00%
43) trans-1,3-Dichloroprop...	8.186	79	23590	5.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.80%
46) 2-Hexanone-d5	8.645	63	115246	59.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.70%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	42645	5.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	55313	5.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.80%
Target Compounds						Qvalue
16) Methylene chloride	3.051	84	2727	0.30	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042121.D
Acq On : 20 Jan 2021 21:57
Operator : SY/MD
Sample : VU0120WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK22


Quant Time: Jan 21 06:01:45 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jan 21 06:00:33 2021
Response via : Initial Calibration

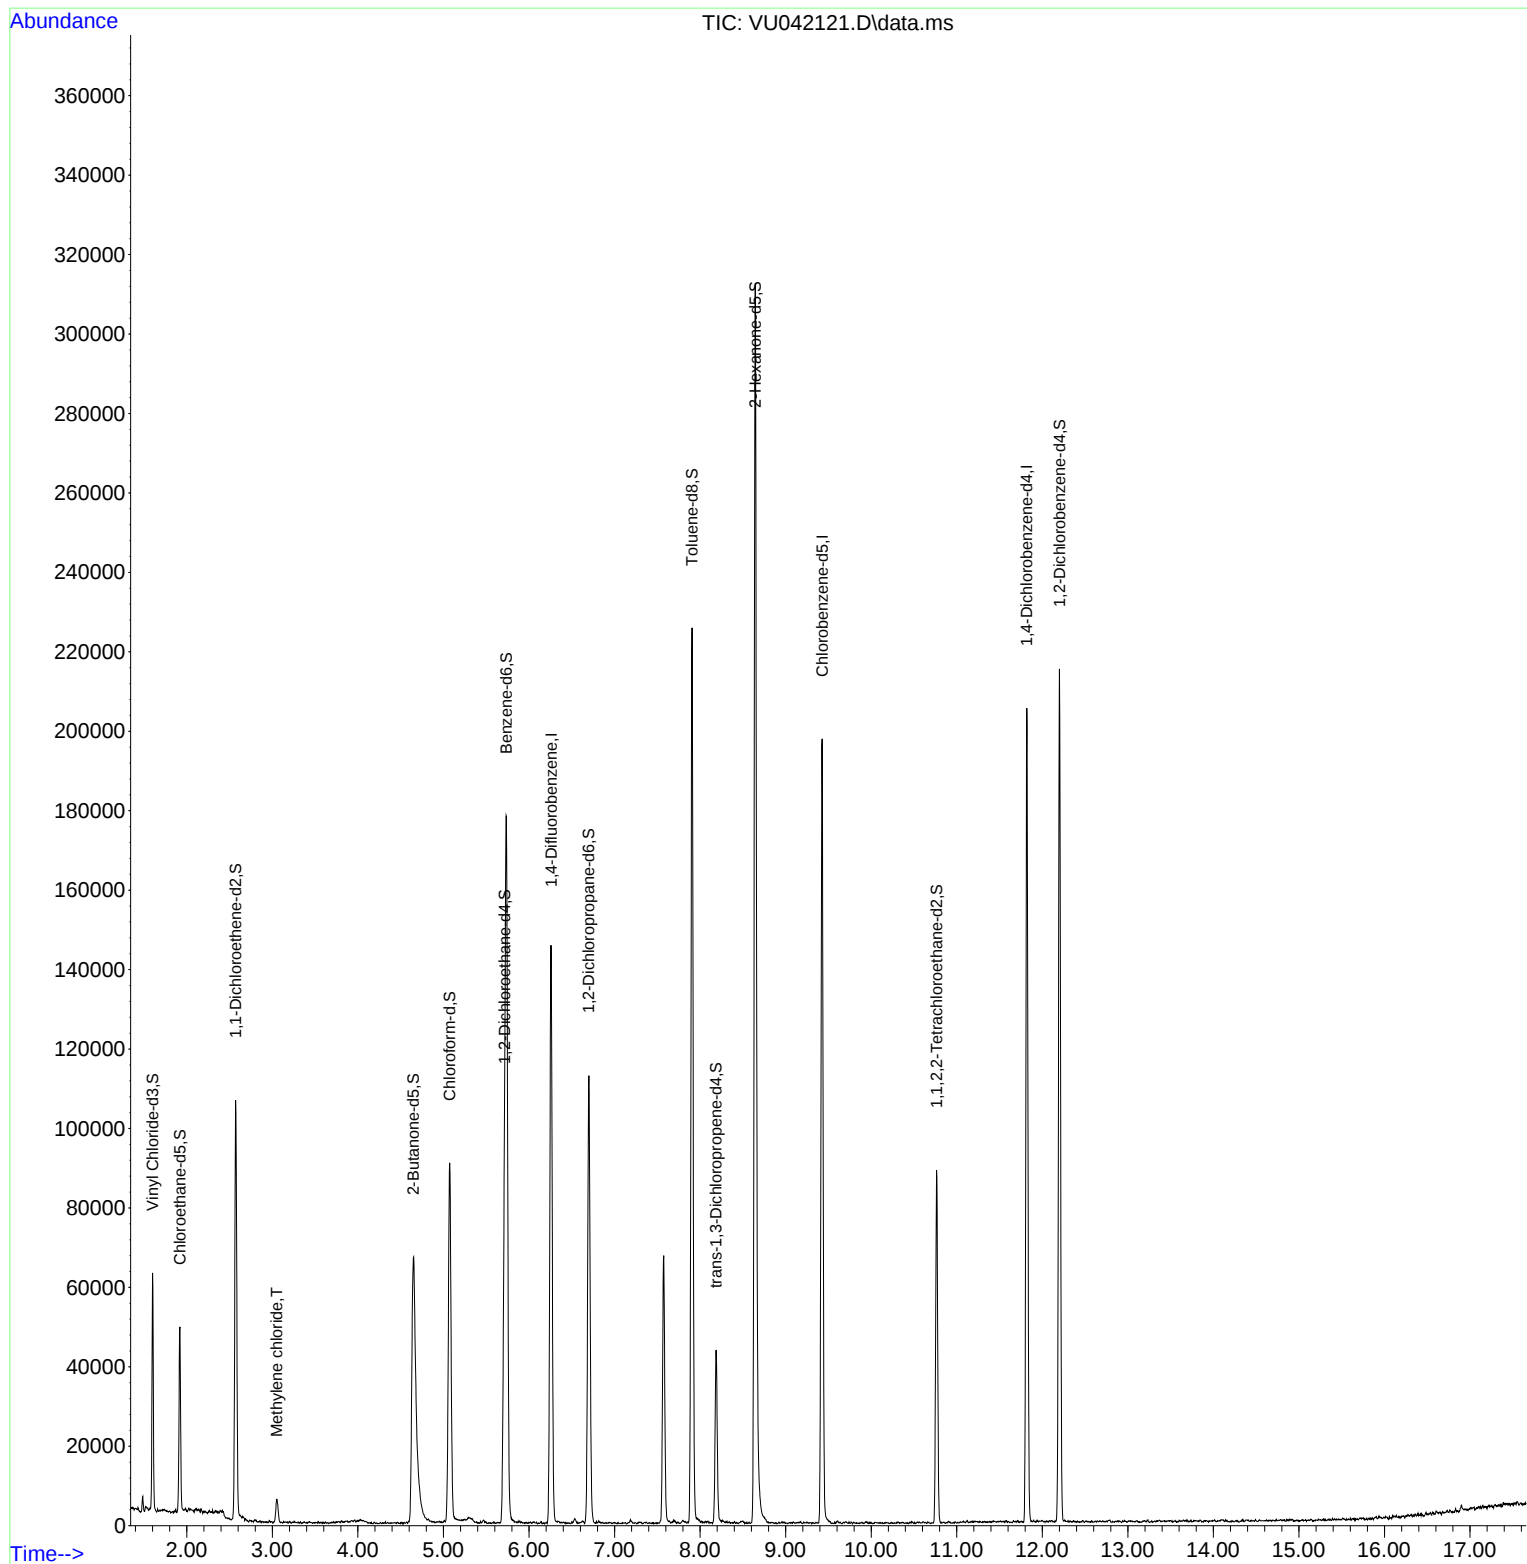

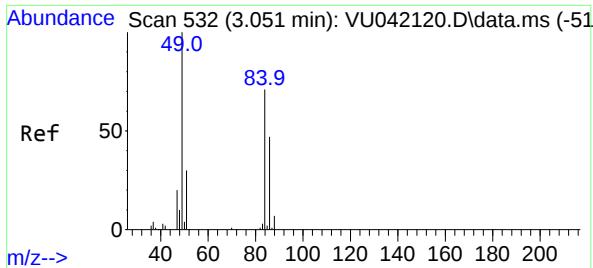

#16
Methylene chloride
Concen: 0.30 ug/L
RT: 3.051 min Scan# 532
Delta R.T. 0.000 min
Lab File: VU042121.D
Acq: 20 Jan 2021 21:57

Instrument :
MSVOA_U
ClientSampleId :
VBLK22

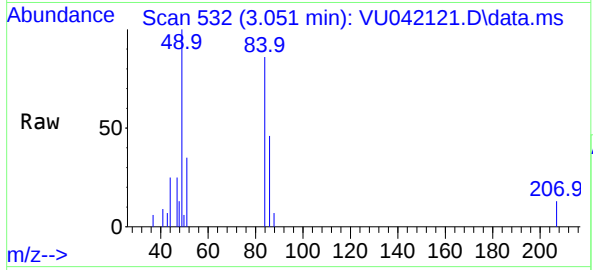

Tgt Ion:	84	Resp:	2727
Ion	Ratio	Lower	Upper
84	100		
86	53.1	44.1	81.9
49	123.4	95.0	176.4

