

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
 Data File : VU042111.D
 Acq On : 20 Jan 2021 17:24
 Operator : SY/MD
 Sample : M1164-01DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXP8DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC: VU042111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	90	rVB	56529	60268	8.76%	1.275%
2	1.916	172	179	191	rVB	44004	56360	8.20%	1.192%
3	2.571	372	383	396	rBV	101026	162320	23.60%	3.434%
4	3.054	523	533	548	rVB3	6755	13650	1.98%	0.289%
5	3.375	619	633	653	rBV2	6505	16309	2.37%	0.345%
6	4.655	1012	1031	1083	rBV2	59583	255537	37.16%	5.406%
7	5.073	1146	1161	1180	rBV	84796	189380	27.54%	4.006%
8	5.735	1346	1367	1391	rBV2	170366	449106	65.31%	9.501%
9	6.256	1515	1529	1550	rBV	156600	296542	43.12%	6.273%
10	6.549	1606	1620	1644	rBV	363795	687659	100.00%	14.547%
11	6.700	1653	1667	1689	rVB	108282	212047	30.84%	4.486%
12	7.574	1925	1939	1958	rBV	64859	117688	17.11%	2.490%
13	7.906	2028	2042	2059	rBV	213310	372718	54.20%	7.885%
14	8.189	2117	2130	2144	rBV	43842	75949	11.04%	1.607%
15	8.562	2237	2246	2257	rVB4	8448	13514	1.97%	0.286%
16	8.645	2257	2272	2314	rBV	276218	569492	82.82%	12.047%
17	9.426	2501	2515	2529	rBV	211039	352787	51.30%	7.463%
18	10.764	2915	2931	2948	rVB	85973	140089	20.37%	2.964%
19	11.822	3244	3260	3277	rBV	219059	354791	51.59%	7.506%
20	12.201	3364	3378	3394	rBV	203480	330852	48.11%	6.999%




Sum of corrected areas: 4727058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042111.D
Acq On : 20 Jan 2021 17:24
Operator : SY/MD
Sample : M1164-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

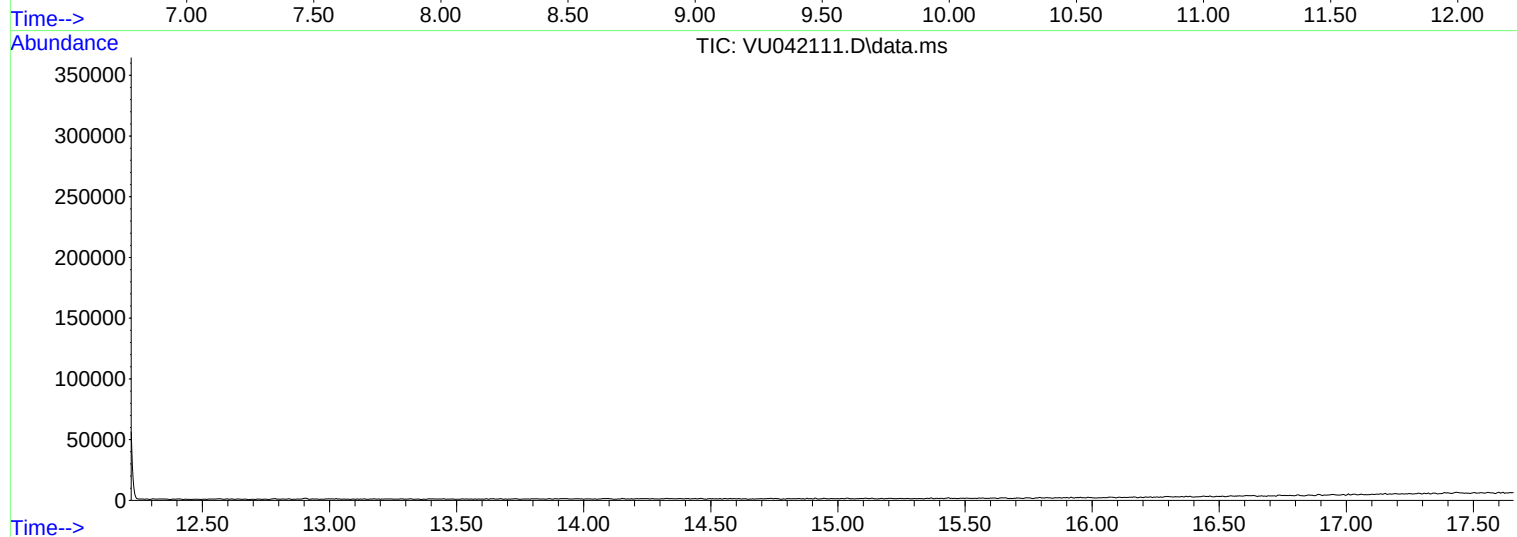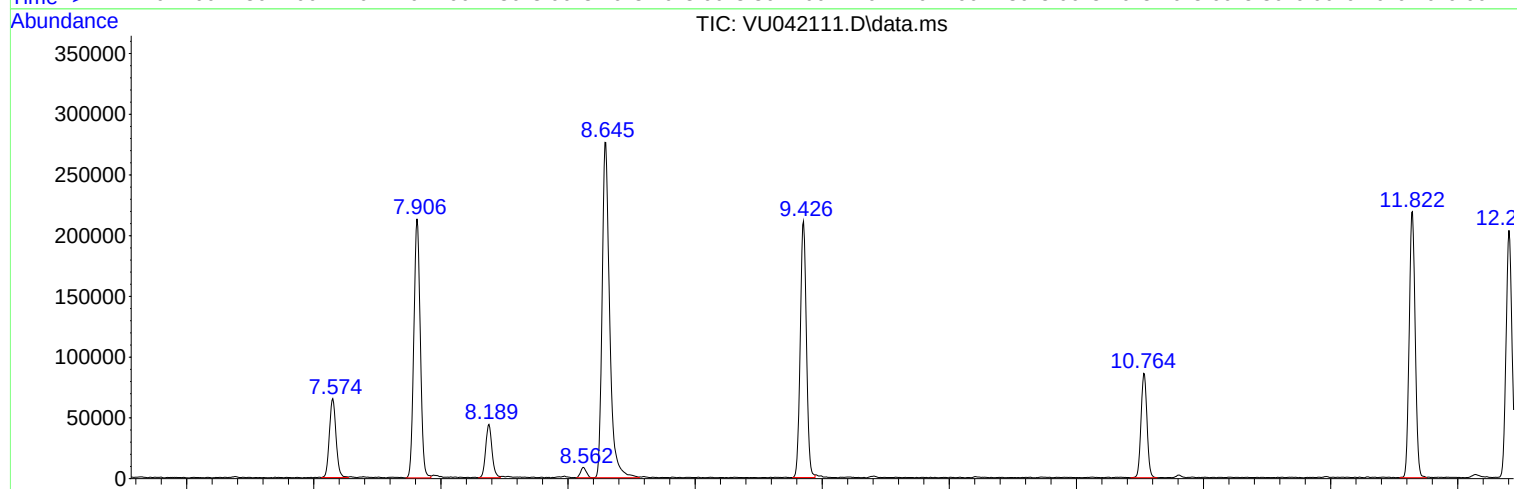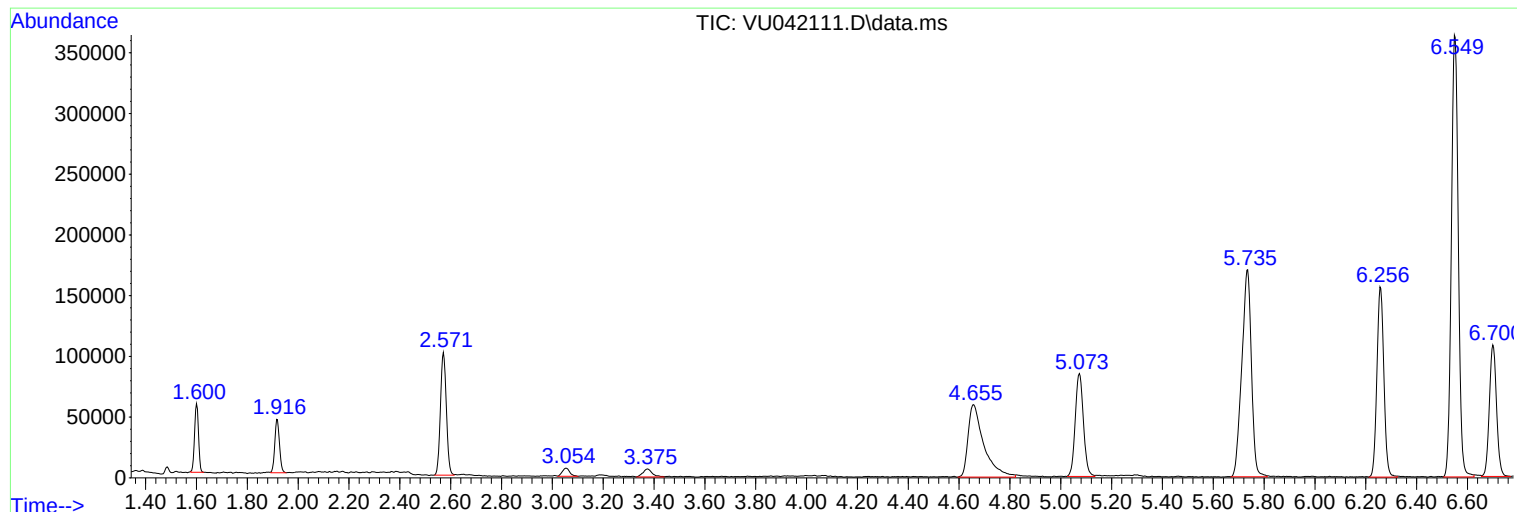

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042111.D
Acq On : 20 Jan 2021 17:24
Operator : SY/MD
Sample : M1164-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042111.D
Acq On : 20 Jan 2021 17:24
Operator : SY/MD
Sample : M1164-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
