

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
 Data File : VU042113.D
 Acq On : 20 Jan 2021 18:12
 Operator : SY/MD
 Sample : M1164-08DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXT5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	92	rBV	56184	60577	9.18%	1.329%
2	1.916	172	179	193	rVB	42732	53304	8.08%	1.170%
3	2.572	371	383	400	rBV	98709	158229	23.99%	3.473%
4	3.054	522	533	547	rBV2	7363	14223	2.16%	0.312%
5	3.375	618	633	651	rBV2	6024	15113	2.29%	0.332%
6	4.655	1014	1031	1079	rBV2	54973	233305	35.37%	5.120%
7	5.073	1146	1161	1181	rBV	82713	185109	28.06%	4.063%
8	5.732	1343	1366	1385	rBV2	166555	439734	66.66%	9.651%
9	6.256	1514	1529	1549	rBV	150190	282696	42.85%	6.204%
10	6.549	1605	1620	1641	rBV	348717	659677	100.00%	14.478%
11	6.700	1653	1667	1686	rVB	106235	206452	31.30%	4.531%
12	7.575	1922	1939	1955	rBV	62798	112937	17.12%	2.479%
13	7.906	2026	2042	2059	rBV	212018	364422	55.24%	7.998%
14	8.189	2115	2130	2144	rBV2	41188	72340	10.97%	1.588%
15	8.558	2236	2245	2254	rVB2	7723	12127	1.84%	0.266%
16	8.645	2257	2272	2314	rBV	277491	548721	83.18%	12.043%
17	9.423	2500	2514	2531	rBV	201899	340058	51.55%	7.463%
18	10.764	2920	2931	2949	rVB	83296	135489	20.54%	2.974%
19	11.819	3245	3259	3278	rVB	209618	338112	51.25%	7.420%
20	12.201	3364	3378	3399	rVB	198727	323838	49.09%	7.107%




Sum of corrected areas: 4556463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042113.D
Acq On : 20 Jan 2021 18:12
Operator : SY/MD
Sample : M1164-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXT5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

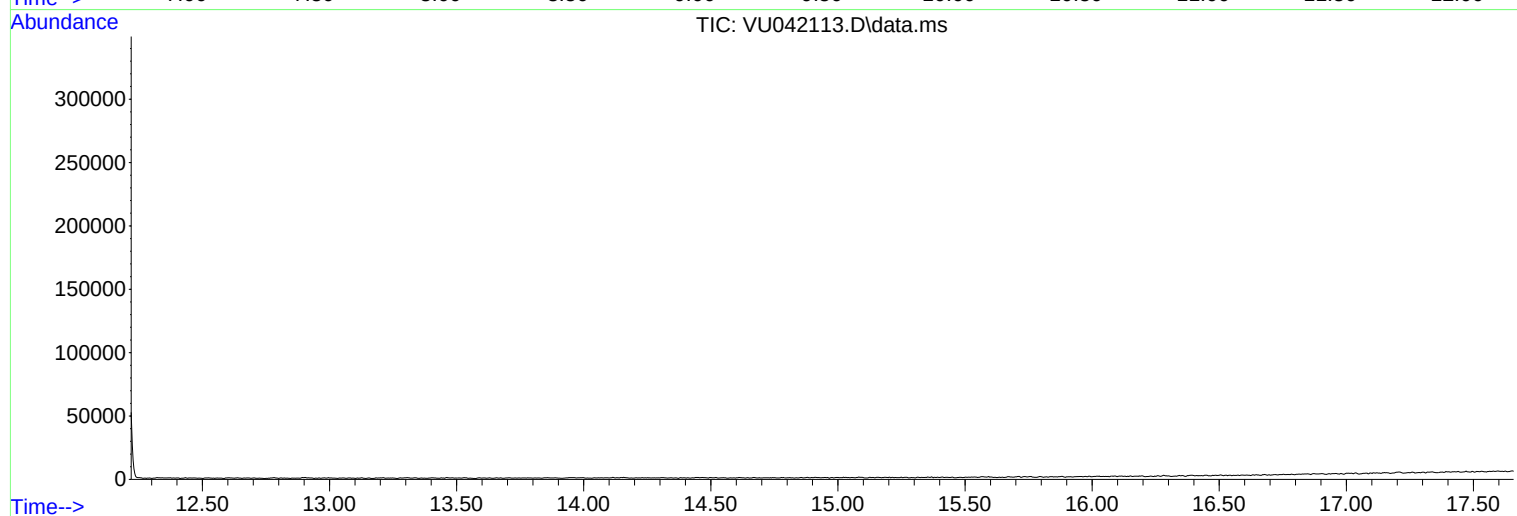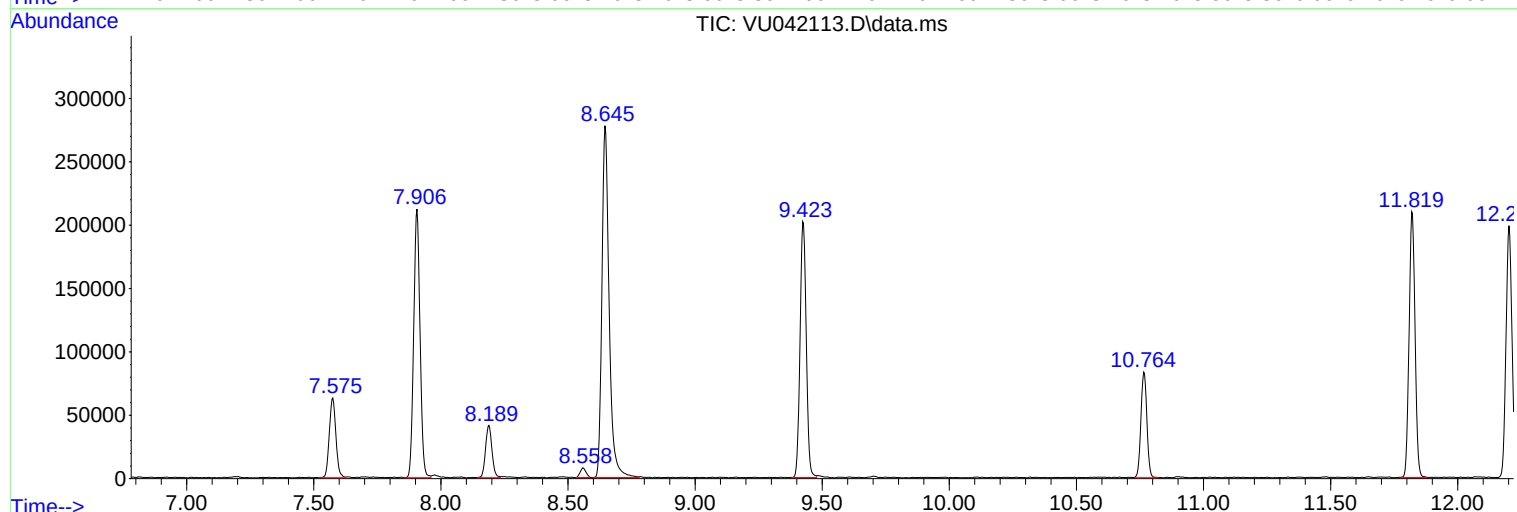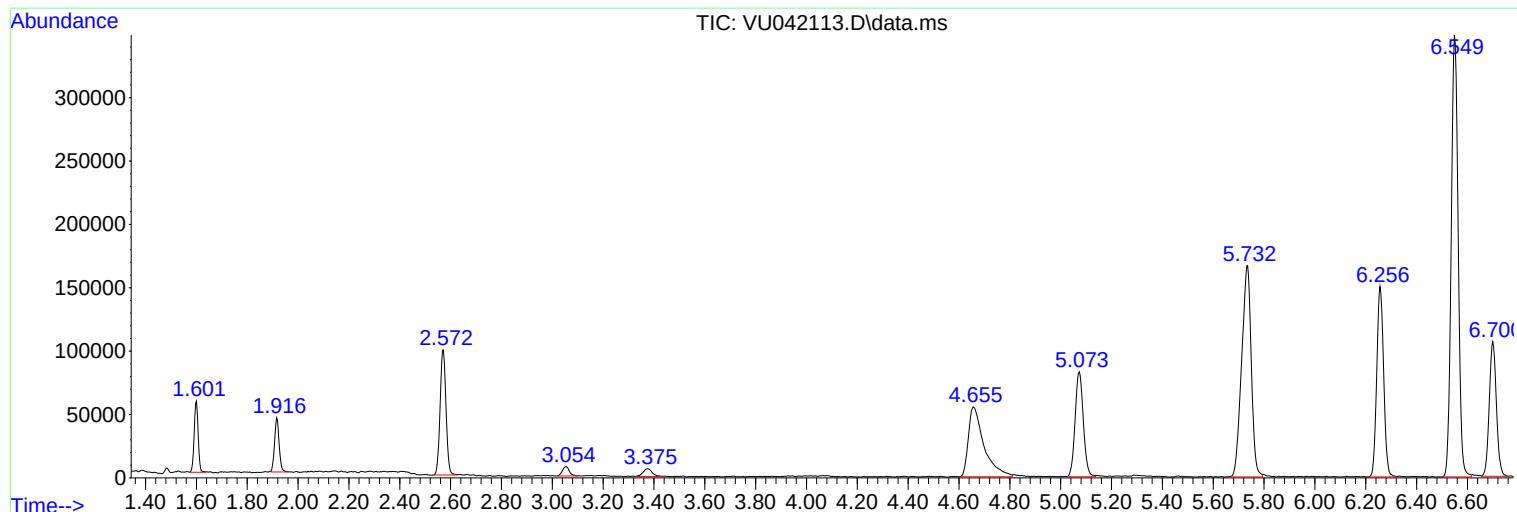

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042113.D
Acq On : 20 Jan 2021 18:12
Operator : SY/MD
Sample : M1164-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXT5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
Data File : VU042113.D
Acq On : 20 Jan 2021 18:12
Operator : SY/MD
Sample : M1164-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXT5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
