


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012021\
 Data File : VU042094.D
 Acq On : 20 Jan 2021 09:23
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 23 06:18:59 2021

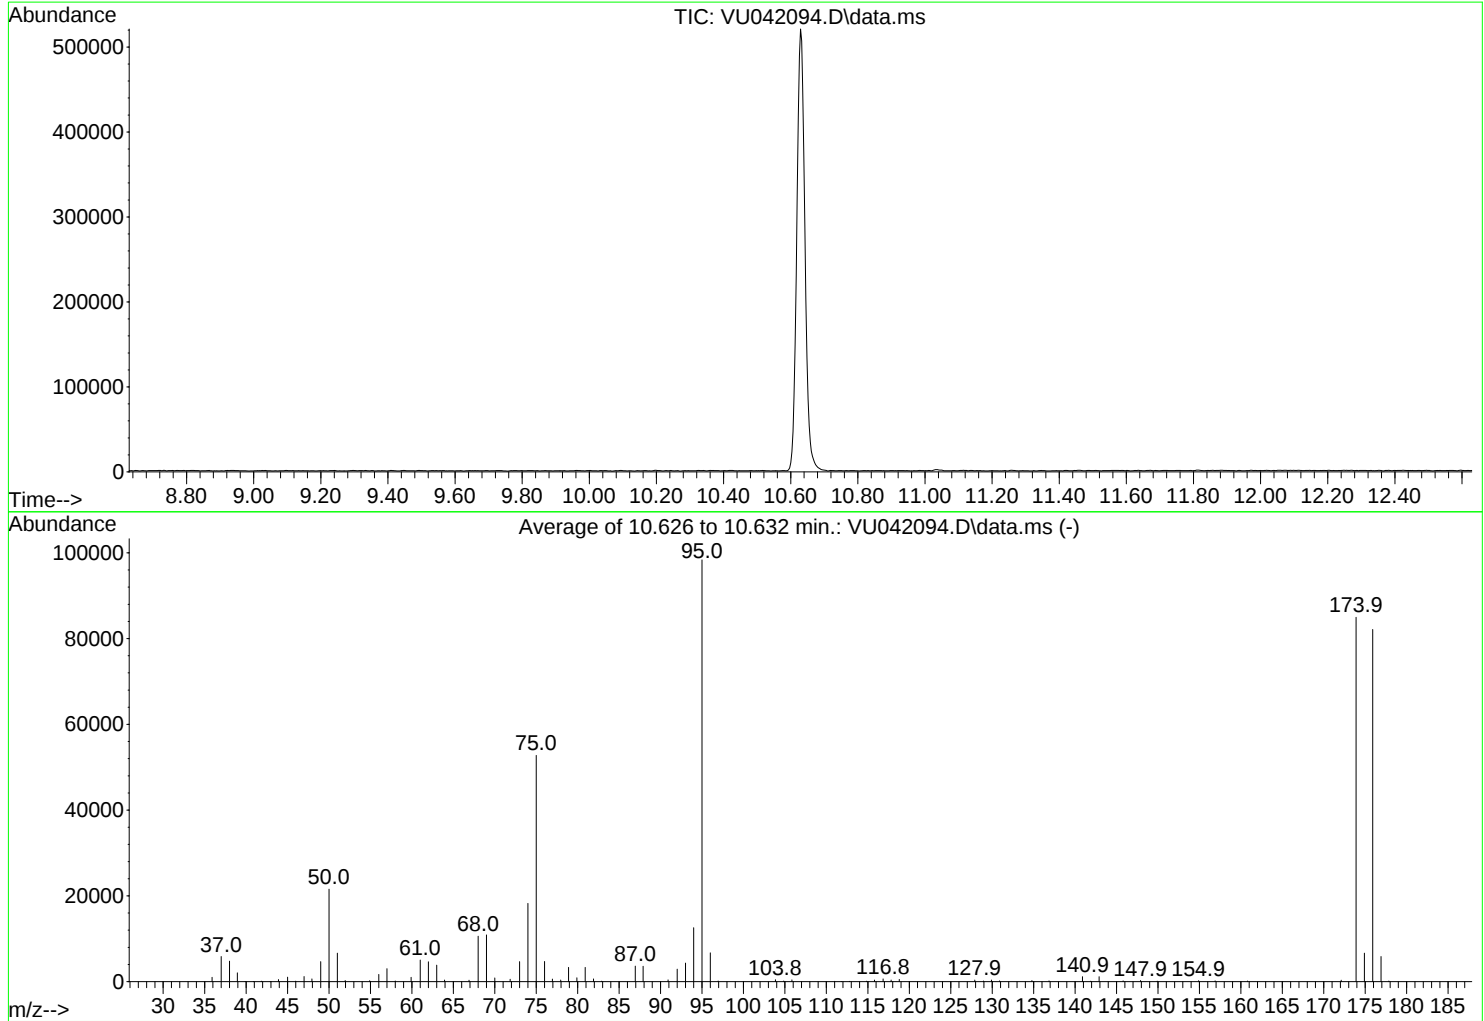

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	21571	PASS
75	95	30	80	53.7	52779	PASS
95	95	100	100	100.0	98368	PASS
96	95	5	9	6.8	6729	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.4	84973	PASS
175	174	5	9	7.8	6628	PASS
176	174	95	101	96.7	82136	PASS
177	176	5	9	7.2	5876	PASS

m/z	Abundance
38.90	104.0
39.90	119.0
41.00	142.0
42.90	150.0
43.90	522.0
54.90	134.0
206.90	385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	961.0
37.00	5808.0
38.00	4819.0
39.00	2013.0
39.90	169.0
40.90	170.0
41.90	117.0
42.90	157.0
44.00	954.0
45.00	1057.0
46.00	100.0
47.00	1171.0
48.00	633.0
49.00	4619.0
50.00	21216.0
51.00	6542.0
51.90	258.0
55.00	362.0
56.00	1681.0
57.00	2898.0
58.00	161.0
59.90	992.0
61.00	4984.0
62.00	4498.0
63.00	3778.0
64.00	397.0
66.90	325.0
68.00	10347.0
69.00	10660.0
70.00	870.0
71.90	589.0
73.00	4509.0
74.00	17712.0
75.00	51880.0
76.00	4712.0
76.90	602.0
78.00	368.0
78.90	3179.0
79.90	922.0
80.90	3215.0
81.90	604.0
82.90	105.0
86.90	3629.0
87.90	3645.0
90.90	396.0
92.00	2727.0
93.00	4035.0
94.00	12027.0
95.00	95208.0
96.00	6655.0
96.90	155.0
103.80	440.0
104.80	169.0
105.90	383.0
111.00	117.0
112.80	110.0
114.90	149.0
115.80	409.0
116.80	598.0
117.80	344.0
118.80	519.0
127.90	375.0
128.90	156.0
129.90	340.0
130.90	191.0
134.80	262.0
136.80	160.0
140.90	1082.0
141.90	102.0
142.90	1095.0
145.80	162.0
147.80	258.0
149.90	111.0
154.90	241.0
156.90	179.0
160.80	156.0
172.10	306.0
173.90	80960.0
174.90	6359.0
175.90	78104.0
176.90	5767.0
177.80	173.0
207.00	308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	1023.0
37.00	6069.0
38.00	4880.0
39.00	2214.0
39.90	164.0
40.90	166.0
41.80	126.0
42.90	156.0
43.90	1012.0
45.00	1089.0
46.00	118.0
47.00	1222.0
47.90	647.0
49.00	4779.0
50.00	22224.0
51.00	6866.0
52.00	288.0
54.90	388.0
56.00	1754.0
57.00	3136.0
58.00	153.0
59.90	1052.0
61.00	5230.0
62.00	4740.0
63.00	3931.0
64.00	373.0
66.90	336.0
68.00	10939.0
69.00	11301.0
70.00	884.0
71.90	582.0
73.00	4762.0
74.00	18800.0
75.00	54320.0
76.00	4866.0
76.90	633.0
78.00	357.0
78.90	3412.0
79.90	950.0
80.90	3482.0
81.90	660.0
82.90	134.0
87.00	3715.0
87.90	3692.0
90.90	417.0
92.00	3028.0
93.00	4490.0
94.00	13009.0
95.00	101072.0
96.00	6890.0
96.90	145.0
103.80	469.0
104.90	178.0
105.80	416.0
111.00	118.0
112.80	103.0
114.80	127.0
115.80	409.0
116.90	667.0
117.80	393.0
118.80	532.0
127.90	368.0
128.90	161.0
129.90	367.0
130.90	201.0
134.80	269.0
136.90	184.0
140.90	1202.0
141.90	127.0
142.90	1193.0
145.80	196.0
147.90	253.0
149.90	110.0
154.90	225.0
156.90	193.0
160.80	158.0
172.10	361.0
173.90	87632.0
174.90	6827.0
175.90	84552.0
176.90	6074.0
177.90	135.0
206.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	1025.0
37.00	5687.0
38.00	4623.0
39.00	2194.0
39.90	156.0
40.90	172.0
41.80	112.0
42.90	161.0
43.90	1049.0
45.00	1002.0
46.00	105.0
47.00	1169.0
47.90	660.0
49.00	4572.0
50.00	21272.0
51.00	6523.0
52.00	296.0
54.90	382.0
56.00	1603.0
57.00	3053.0
58.00	151.0
59.90	982.0
61.00	4941.0
62.00	4697.0
63.00	3800.0
63.90	341.0
66.90	306.0
68.00	10559.0
69.00	10768.0
70.00	833.0
71.80	531.0
73.00	4717.0
74.00	18192.0
75.00	52136.0
76.00	4575.0
77.00	578.0
77.90	364.0
78.90	3320.0
79.90	850.0
80.90	3288.0
81.90	698.0
82.90	145.0
86.90	3519.0
87.90	3388.0
90.90	405.0
92.00	2974.0
93.00	4517.0
94.00	12657.0
95.00	98824.0
96.00	6642.0
97.00	155.0
103.90	481.0
104.90	158.0
105.80	410.0
111.80	100.0
114.80	115.0
115.80	361.0
116.90	688.0
117.80	414.0
118.80	534.0
127.90	368.0
129.00	152.0
129.90	378.0
130.90	178.0
134.80	249.0
136.90	191.0
140.90	1232.0
141.90	136.0
142.90	1141.0
145.80	184.0
148.00	239.0
149.90	110.0
154.90	212.0
156.90	198.0
160.80	140.0
172.10	334.0
173.90	86328.0
174.90	6699.0
175.90	83752.0
176.90	5786.0
177.90	105.0
206.90	306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38