


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012023\
Data File : VU052750.D
Acq On : 20 Jan 2023 09:36
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U011923W.M
Title : SW846 8260
Last Update : Fri Jan 20 01:04:16 2023

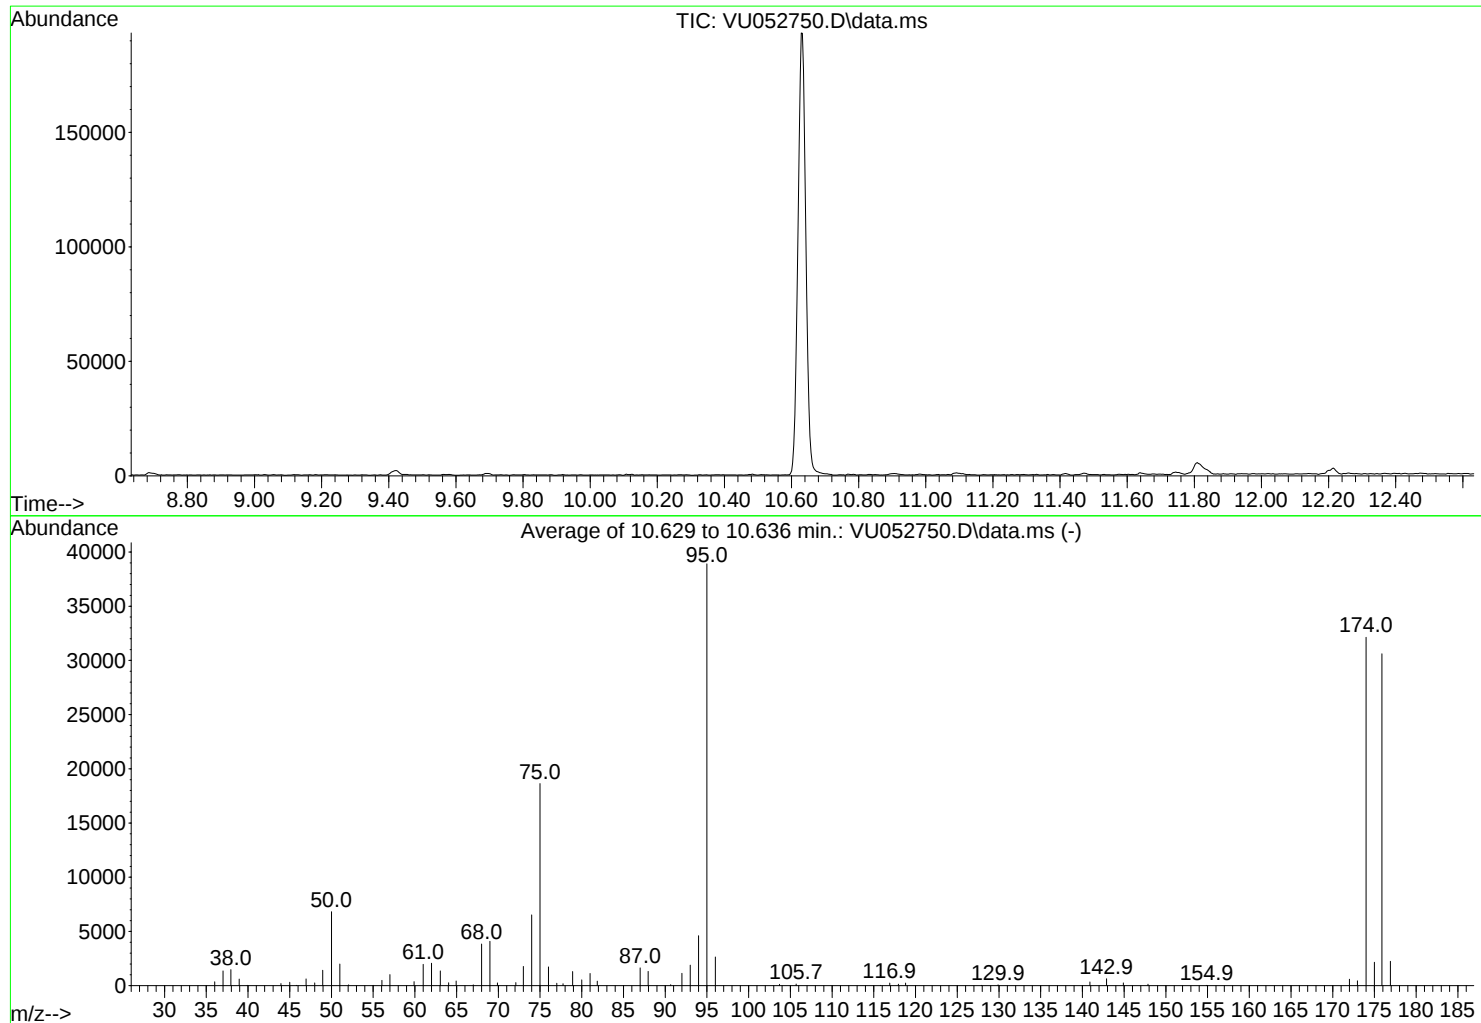

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6817	PASS
75	95	30	60	47.9	18648	PASS
95	95	100	100	100.0	38909	PASS
96	95	5	9	6.8	2637	PASS
173	174	0.00	2	1.4	438	PASS
174	95	50	100	82.6	32136	PASS
175	174	5	9	6.7	2152	PASS
176	174	95	101	95.3	30611	PASS
177	176	5	9	7.3	2246	PASS