
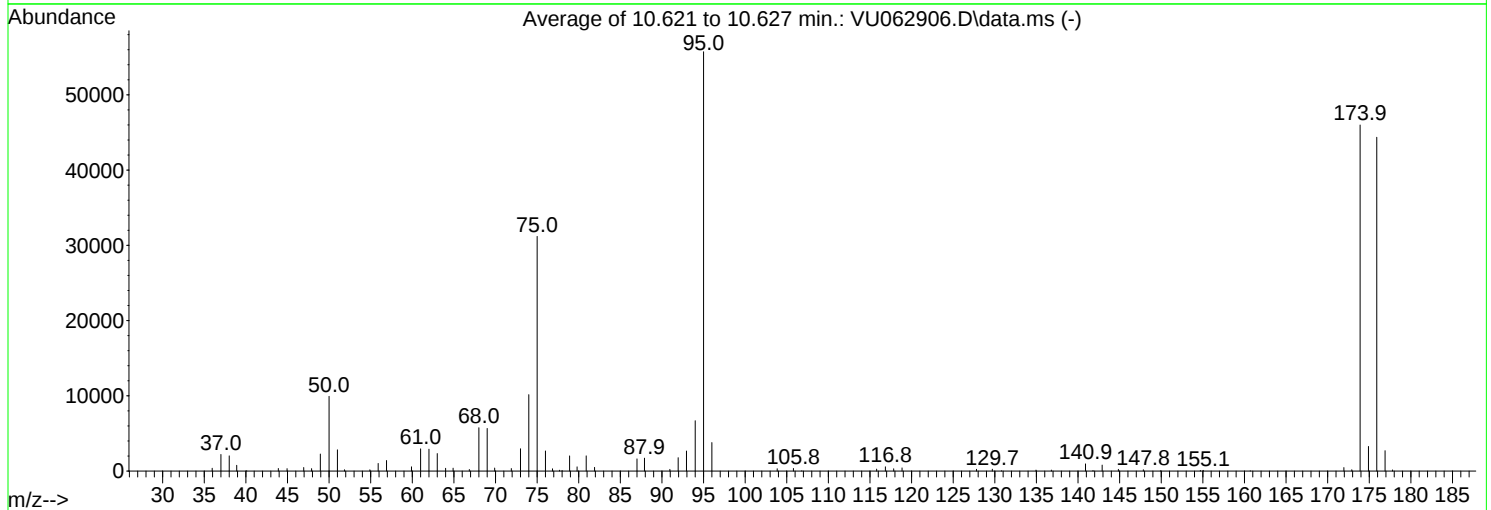


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012025\
Data File : VU062906.D
Acq On : 20 Jan 2025 09:14
Operator : MD/SY
Sample : BFB064
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB064

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 23 00:43:08 2025

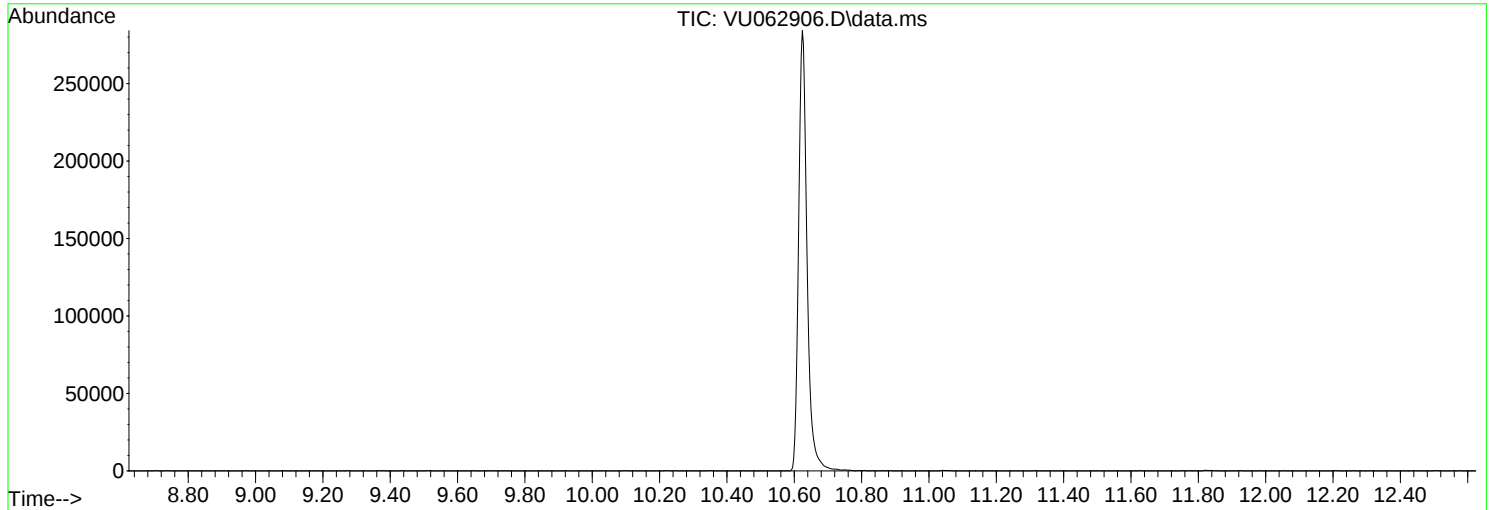

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9933	PASS
75	95	30	80	56.0	31189	PASS
95	95	100	100	100.0	55731	PASS
96	95	5	9	6.8	3789	PASS
173	174	0.00	2	0.4	180	PASS
174	95	50	120	82.5	45995	PASS
175	174	5	9	7.1	3277	PASS
176	174	95	101	96.5	44363	PASS
177	176	5	9	6.1	2710	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB064

m/z	Abundance
35.90	385.0
37.00	2260.0
38.00	2121.0
38.90	798.0
40.10	119.0
43.90	348.0
45.00	320.0
47.00	372.0
47.90	289.0
48.90	2118.0
50.00	9944.0
51.00	2835.0
51.90	173.0
54.90	115.0
55.90	1026.0
56.90	1345.0
59.90	626.0
61.00	2904.0
62.00	2892.0
63.00	2195.0
64.00	387.0
64.90	309.0
66.90	227.0
68.00	5509.0
69.00	5517.0
69.90	397.0
71.90	345.0
73.00	2720.0
74.00	9755.0
75.00	30744.0
76.00	2676.0
76.90	329.0
78.00	186.0
78.90	1946.0
79.80	572.0
80.90	2159.0
81.90	448.0
87.00	1490.0
87.90	1899.0
91.00	194.0
92.00	1733.0
92.90	2516.0
94.00	6490.0
95.00	54160.0
96.00	3749.0
103.90	288.0
105.70	365.0
115.80	274.0
116.90	554.0
117.80	318.0
118.90	438.0
127.80	241.0
129.70	208.0
135.00	129.0
136.80	161.0
140.90	849.0
141.80	127.0
142.90	800.0
144.80	170.0
147.80	125.0
154.70	126.0
172.00	450.0
173.90	44408.0
174.90	3222.0
175.90	42568.0
176.90	2779.0
177.80	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	378.0
37.00	2245.0
38.00	2095.0
38.90	773.0
43.90	359.0
44.90	339.0
47.00	496.0
47.90	357.0
48.90	2293.0
50.00	10291.0
51.00	2866.0
51.80	194.0
54.90	177.0
55.90	1043.0
56.90	1452.0
59.90	586.0
61.00	3077.0
62.00	3019.0
63.00	2397.0
64.00	391.0
64.90	386.0
66.90	232.0
68.00	5865.0
69.00	5806.0
69.90	417.0
71.90	336.0
73.00	3046.0
74.00	10432.0
75.00	32264.0
76.00	2812.0
76.90	297.0
77.70	153.0
78.90	2094.0
79.80	587.0
80.90	2065.0
81.90	495.0
87.00	1649.0
87.90	1778.0
91.00	237.0
92.00	1820.0
93.00	2713.0
94.00	6874.0
95.00	57240.0
96.00	3960.0
103.80	322.0
105.80	353.0
115.80	271.0
116.80	595.0
117.90	297.0
118.80	416.0
127.80	253.0
129.70	258.0
134.90	144.0
136.80	142.0
140.90	1004.0
141.80	107.0
142.90	795.0
144.80	248.0
147.90	171.0
154.70	118.0
155.10	117.0
172.00	479.0
173.90	47568.0
174.90	3380.0
175.90	45792.0
176.90	2784.0
177.80	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
36.00	362.0
37.00	2121.0
38.00	1850.0
38.90	722.0
43.90	334.0
44.90	318.0
46.90	547.0
47.90	342.0
49.00	2382.0
50.00	9563.0
51.00	2775.0
51.80	170.0
54.90	227.0
55.90	977.0
56.90	1418.0
59.90	491.0
61.00	2885.0
62.00	2829.0
63.00	2399.0
64.00	338.0
64.90	481.0
66.80	170.0
68.00	5905.0
69.00	5667.0
69.90	385.0
71.90	337.0
73.00	3138.0
74.00	10277.0
75.00	30560.0
76.00	2543.0
76.80	297.0
77.70	188.0
78.90	2006.0
79.80	532.0
80.90	1842.0
81.90	526.0
87.00	1718.0
87.90	1473.0
90.90	267.0
91.90	1787.0
93.00	2770.0
94.00	6706.0
95.00	55792.0
96.00	3659.0
103.90	328.0
105.90	326.0
106.80	110.0
115.80	237.0
116.90	551.0
117.80	297.0
118.80	422.0
127.80	222.0
129.70	272.0
130.80	132.0
134.90	133.0
136.80	109.0
140.90	1015.0
142.90	804.0
144.90	265.0
147.90	242.0
149.90	107.0
155.00	168.0
160.70	108.0
171.90	473.0
172.90	539.0
173.90	46008.0
174.90	3230.0
175.90	44728.0
176.90	2567.0
177.80	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064