

Data File : VU029256.D
Acq On : 21 Jan 2019 18:08
Operator : JC/SP
Sample : K1009-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A

Quant Time: Jan 22 01:15:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Sat Jan 12 01:33:59 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	109821	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	193587	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	184876	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	75598	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	74388	54.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.58%	
35) Dibromofluoromethane	4.88	113	64863	51.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.38%	
50) Toluene-d8	7.56	98	251822	50.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.66%	
62) 4-Bromofluorobenzene	10.30	95	77774	43.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.36%	


Target Compounds			Qvalue			
3) Chloromethane	1.33	50	705	Below Cal		97
11) Tert butyl alcohol	2.83	59	118	0.342 ug/l #		73
16) Acetone	2.32	43	8195	9.582 ug/l		97
17) Carbon Disulfide	2.48	76	254	Below Cal #		75
18) Methyl Acetate	2.62	43	1864	0.937 ug/l #		79
20) Methylene Chloride	2.70	84	8553	5.890 ug/l		96
25) 2-Butanone	4.29	43	623	0.539 ug/l #		47
29) Tetrahydrofuran	4.67	42	303	0.432 ug/l #		30
31) Cyclohexane	4.99	56	2047	Below Cal #		1
36) 1,1-Dichloropropene	4.98	75	8270	4.274 ug/l #		47
37) Ethyl Acetate	4.29	43	623	0.293 ug/l #		66
38) Carbon Tetrachloride	4.98	117	9600	5.948 ug/l #		17
43) Isopropyl Acetate	5.55	43	7049	2.164 ug/l #		87
45) 1,2-Dichloropropane	6.70	63	616	0.386 ug/l #		43
48) Methyl methacrylate	6.70	41	39544	24.926 ug/l #		36
51) 4-Methyl-2-Pentanone	7.42	43	35727	16.112 ug/l #		43
54) cis-1,3-Dichloropropene	7.42	75	18539	7.613 ug/l #		60
57) 1,3-Dichloropropane	8.41	76	3597	1.428 ug/l #		42
59) 2-Hexanone	8.31	43	6146	3.531 ug/l #		21
68) m/p-Xylenes	9.38	106	546	0.203 ug/l		80
76) 1,2,3-Trichloropropane	10.30	75	38443	20.755 ug/l #		35
80) 1,3,5-Trimethylbenzene	10.77	105	2429	0.520 ug/l		97
81) trans-1,4-Dichloro-2-buten	10.30	75	38443	53.527 ug/l #		100
84) 1,2,4-Trimethylbenzene	11.15	105	5411	1.160 ug/l		98
90) Hexachloroethane	12.26	117	278	0.348 ug/l #		7
95) Naphthalene	13.74	128	31396	5.367 ug/l		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU029256.D
Acq On : 21 Jan 2019 18:08
Operator : JC/SP
Sample : K1009-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A

Quant Time: Jan 22 01:15:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Sat Jan 12 01:33:59 2019
Response via : Initial Calibration

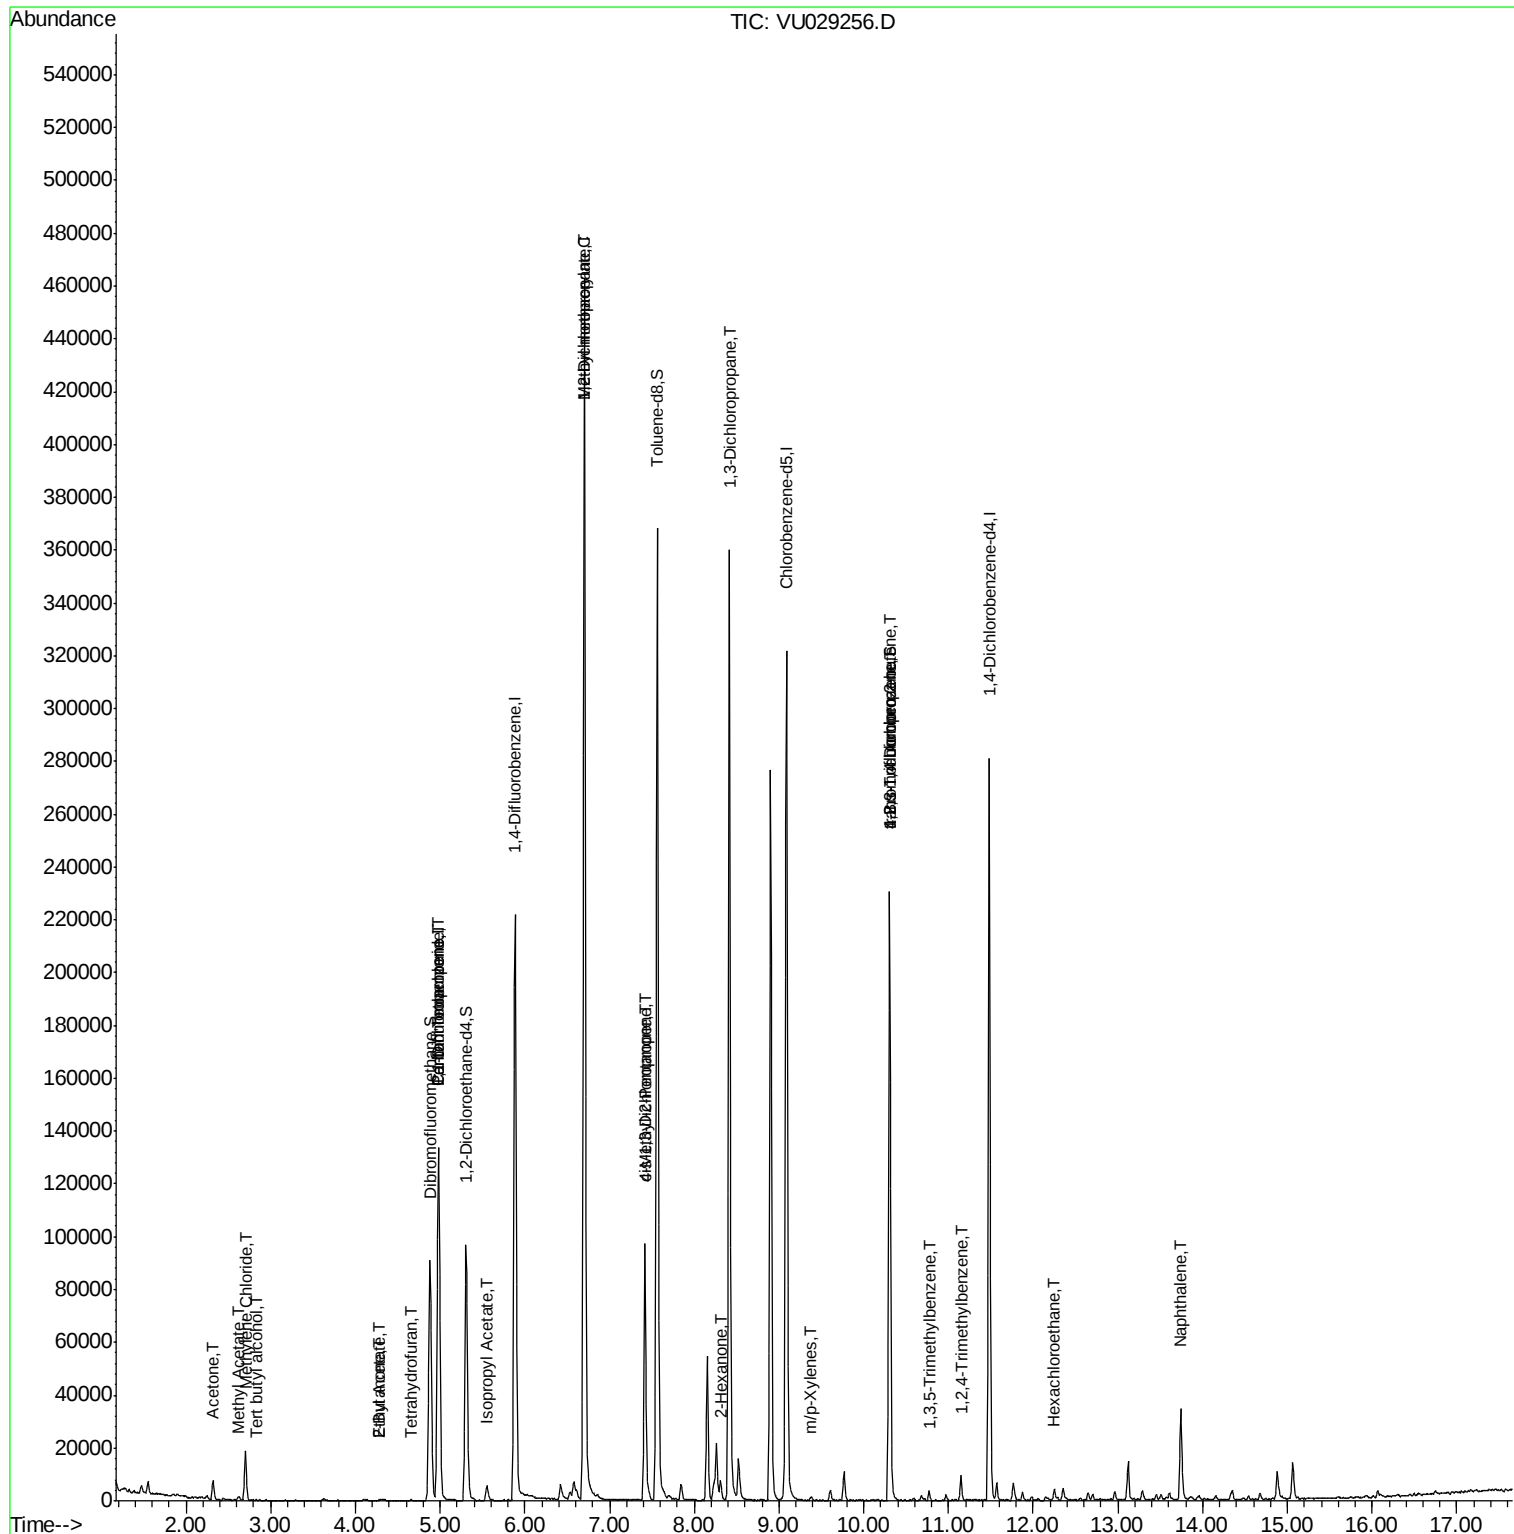

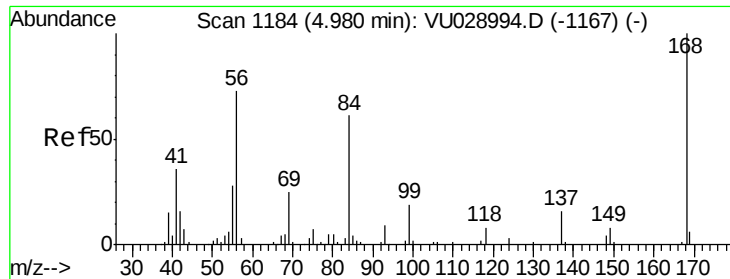

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. 0.00 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :


CL-01-011819-A

Tgt Ion:168 Resp: 109821

Ion Ratio Lower Upper

168 100

99 52.9 42.0 63.0



Abundance Ion 167.90 (167.60 to 168.60): VU028994.D (-1167) (-)

Ion 98.90 (98.60 to 99.60): VU028994.D (-1167) (-)

4.98

50000

40000

30000

20000

10000



0

4.90

5.00

5.10

Time-->



#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 48

Delta R.T. 0.00 min

Lab File: VU029256.D


Acq: 21 Jan 2019 18:08

Tgt Ion: 50 Resp: 705

Ion Ratio Lower Upper

50 100

52 34.0 26.1 39.1



Abundance Ion 49.90 (49.60 to 50.60): VU028994.D (-39) (-)

Ion 51.90 (51.60 to 52.60): VU028994.D (-39) (-)

1.33

600

500

400

300

200

100

0


1.30


1.32

1.34

1.36

Time-->



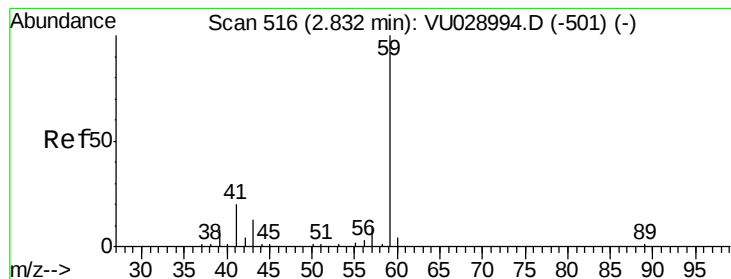

#11

Tert butyl alcohol

Concen: 0.342 ug/l

RT: 2.83 min Scan# 515

Delta R.T. -0.00 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :


CL-01-011819-A

Tgt Ion: 59 Resp: 118

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#



Abundance Ion 59.00 (58.70 to 59.70): VU028994.D (-501) (-)

Ion 57.00 (56.70 to 57.70): VU028994.D (-501) (-)

2.83

150



100

50

0

2.81 2.82 2.83 2.84 2.85

Time-->



#16

Acetone

Concen: 9.582 ug/l

RT: 2.32 min Scan# 357

Delta R.T. 0.00 min

Lab File: VU029256.D


Acq: 21 Jan 2019 18:08

Tgt Ion: 43 Resp: 8195

Ion Ratio Lower Upper

43 100

58 34.0 28.6 42.8



Abundance Ion 43.00 (42.70 to 43.70): VU028994.D (-336) (-)

Ion 58.00 (57.70 to 58.70): VU028994.D (-336) (-)

2.32

5000

4000

3000


2000


1000

0

2.25 2.30 2.35 2.40

Time-->



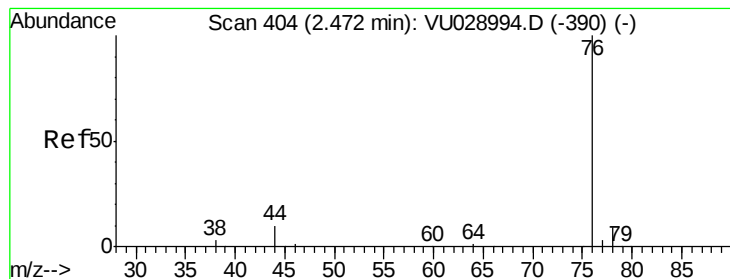

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.48 min Scan# 406

Delta R.T. 0.01 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :


CL-01-011819-A

Tgt Ion: 76 Resp: 254

Ion Ratio Lower Upper




76 100

78 0.0 7.2 10.8#



Abundance Ion 75.90 (75.60 to 76.60): VU0

Ion 77.90 (77.60 to 78.60): VU0

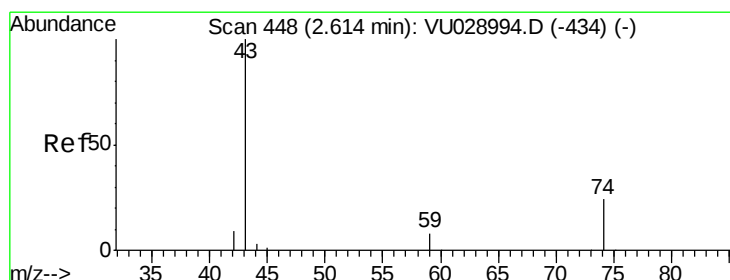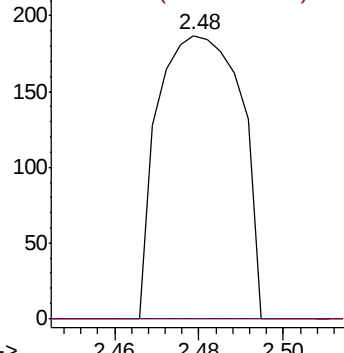

#18

Methyl Acetate

Concen: 0.937 ug/l

RT: 2.62 min Scan# 451

Delta R.T. 0.01 min

Lab File: VU029256.D


Acq: 21 Jan 2019 18:08

Tgt Ion: 43 Resp: 1864

Ion Ratio Lower Upper



43 100


74 13.9 19.5 29.3#



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 74.00 (73.70 to 74.70): VU0




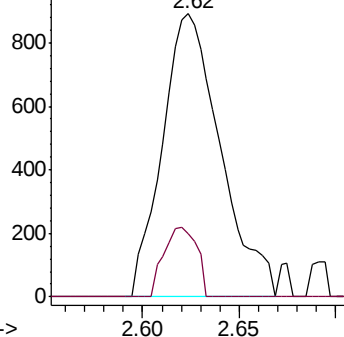


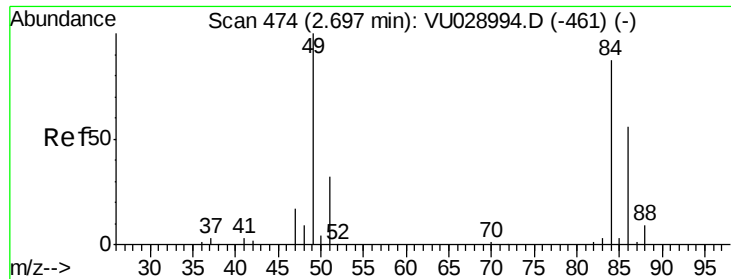

#20
Methylene Chloride
Concen: 5.890 ug/l
RT: 2.70 min Scan# 476
Delta R.T. 0.01 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08




Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A


Tgt Ion:	84	Resp:	8553
Ion	Ratio	Lower	Upper
84	100		
49	110.0	91.9	137.9
51	34.6	29.2	43.8
86	66.4	51.8	77.6

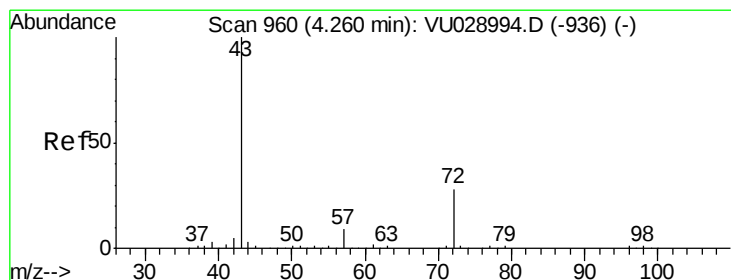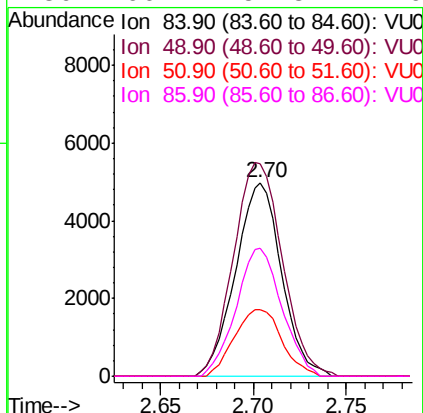

#25
2-Butanone
Concen: 0.539 ug/l
RT: 4.29 min Scan# 969
Delta R.T. 0.03 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08

Tgt Ion:	43	Resp:	623
Ion	Ratio	Lower	Upper
43	100		
72	0.0	22.6	33.8#

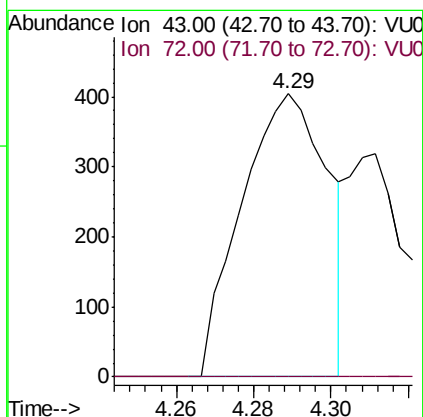



#29

Tetrahydrofuran

Concen: 0.432 ug/l

RT: 4.67 min Scan# 1086

Delta R.T. 0.03 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :

CL-01-011819-A


Tgt Ion: 42 Resp: 303

Ion Ratio Lower Upper

42 100

72 0.0 38.3 57.5#




71 0.0 36.1 54.1#



Abundance Ion 42.00 (41.70 to 42.70): VU0

Ion 72.00 (71.70 to 72.70): VU0

Ion 71.00 (70.70 to 71.70): VU0

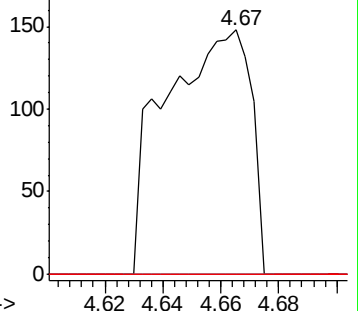

#31

Cyclohexane

Concen: Below Cal

RT: 4.99 min Scan# 1186

Delta R.T. -0.01 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08


Tgt Ion: 56 Resp: 2047

Ion Ratio Lower Upper

56 100

69 182.1 26.7 40.1#



84 162.8 65.7 98.5#




Abundance Ion 56.00 (55.70 to 56.70): VU0

Ion 69.00 (68.70 to 69.70): VU0

Ion 84.00 (83.70 to 84.70): VU0



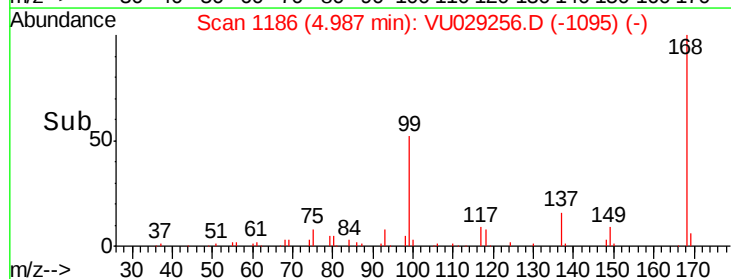
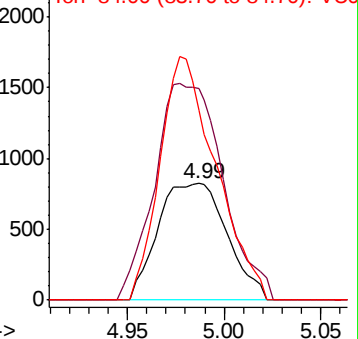


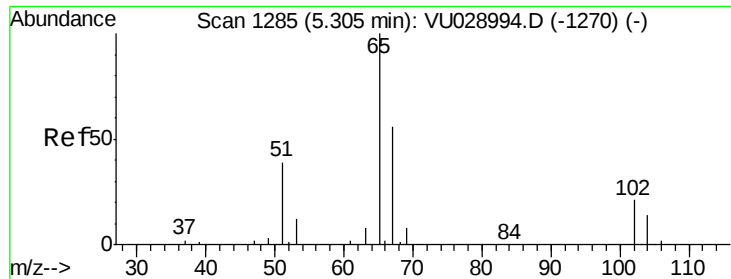

#33
 1,2-Dichloroethane-d4
 Concen: 54.794 ug/l
 RT: 5.31 min Scan# 1286
 Delta R.T. 0.00 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08




Instrument :
 MSVOA_U
 ClientSampleId :
 CL-01-011819-A


Tgt Ion: 65 Resp: 74388
 Ion Ratio Lower Upper
 65 100
 67 56.5 0.0 111.0

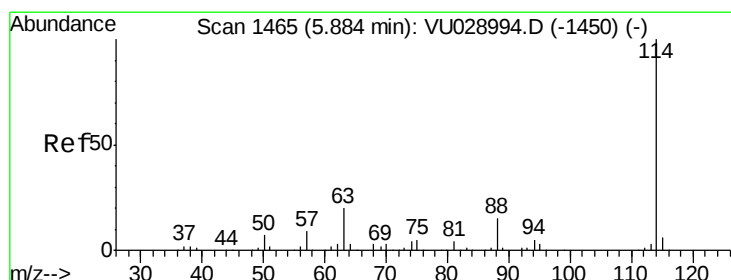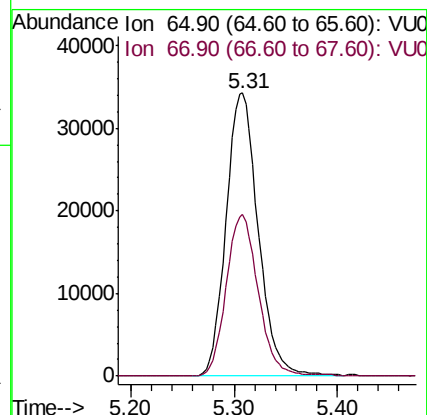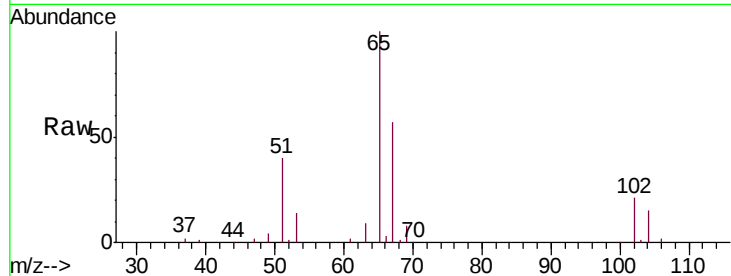

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. -0.00 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08

Tgt Ion: 114 Resp: 193587
 Ion Ratio Lower Upper
 114 100
 63 21.4 0.0 40.2
 88 16.3 0.0 30.4



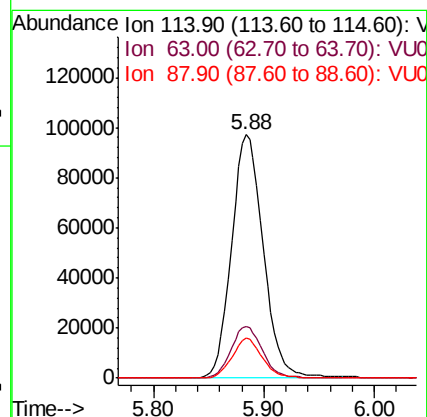





#35
 Dibromofluoromethane
 Concen: 51.688 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. 0.00 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08




Instrument :
 MSVOA_U
 ClientSampleId :
 CL-01-011819-A


Tgt Ion:113 Resp: 64863
 Ion Ratio Lower Upper
 113 100
 111 102.5 81.4 122.2
 192 21.2 16.8 25.2

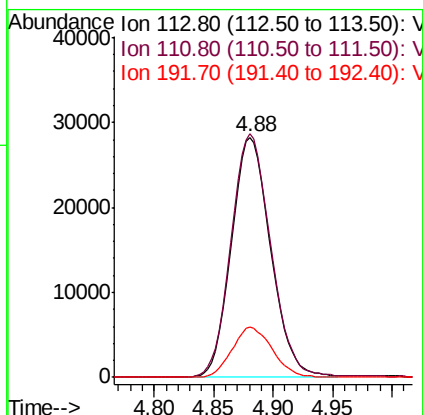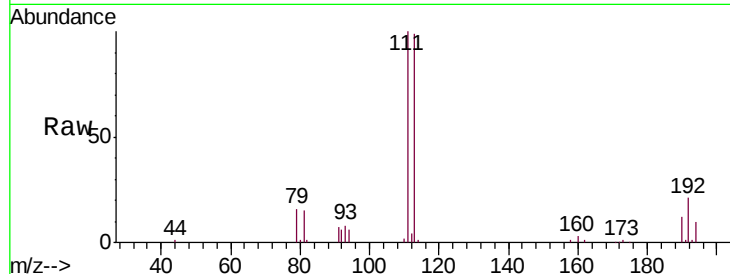

#36
 1,1-Dichloropropene
 Concen: 4.274 ug/l
 RT: 4.98 min Scan# 1184
 Delta R.T. -0.15 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08

Tgt Ion: 75 Resp: 8270
 Ion Ratio Lower Upper
 75 100
 110 7.4 18.4 55.4#
 77 0.0 25.1 37.7#



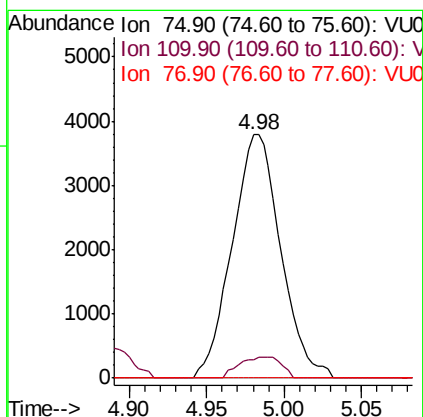
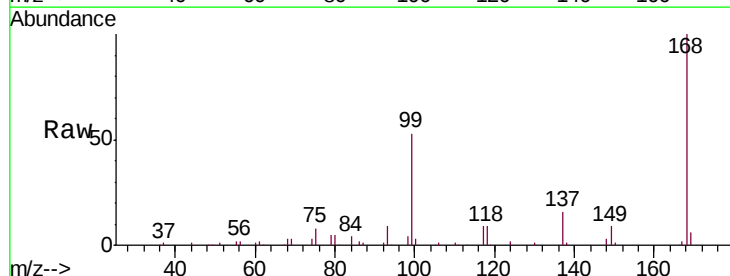




#37
Ethyl Acetate
Concen: 0.293 ug/l
RT: 4.29 min Scan# 969
Delta R.T. -0.09 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08




Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A


Tgt Ion: 43 Resp: 623
Ion Ratio Lower Upper
43 100
61 0.0 12.6 18.8#
70 0.0 9.3 13.9#

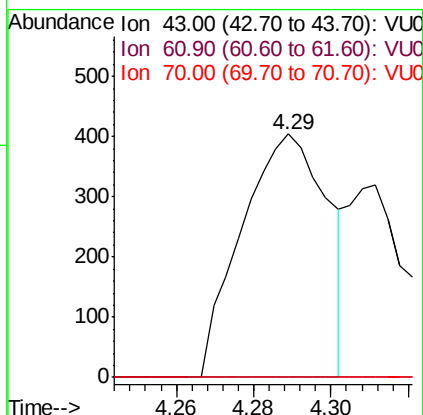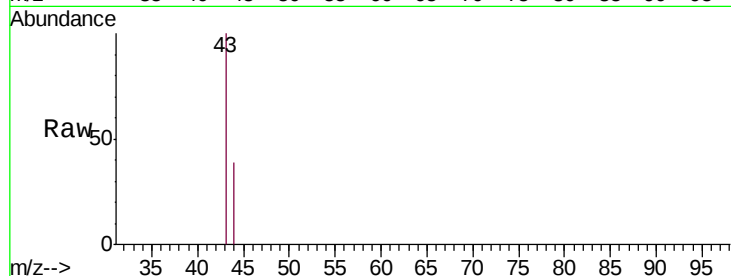

#38
Carbon Tetrachloride
Concen: 5.948 ug/l
RT: 4.98 min Scan# 1185
Delta R.T. -0.15 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08

Tgt Ion: 117 Resp: 9600
Ion Ratio Lower Upper
117 100
119 4.5 74.6 111.8#
121 0.0 25.0 37.6#

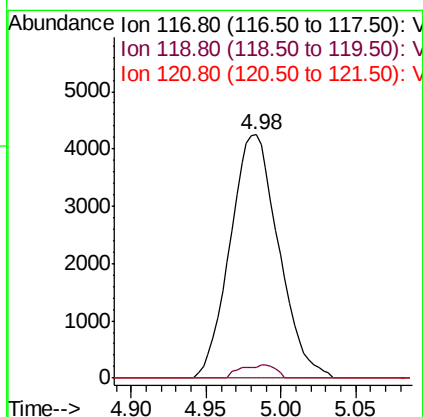



#43

Isopropyl Acetate

Concen: 2.164 ug/l

RT: 5.55 min Scan# 1362

Delta R.T. 0.01 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :

CL-01-011819-A


Tgt Ion: 43 Resp: 7049

Ion Ratio Lower Upper

43 100

61 19.4 17.8 26.6




87 4.2 11.3 16.9#

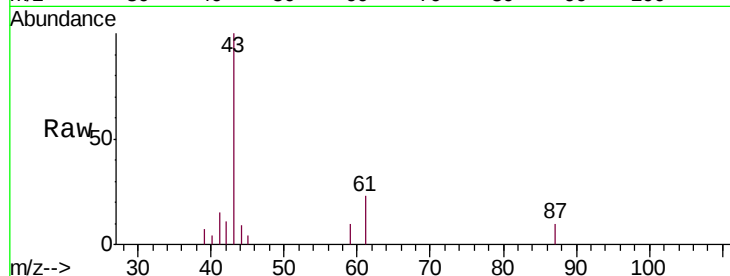

Abundance Ion 43.00 (42.70 to 43.70): VU028994.D (-1342) (-)

Ion 61.00 (60.70 to 61.70): VU028994.D (-1342) (-)

Ion 87.00 (86.70 to 87.70): VU028994.D (-1342) (-)

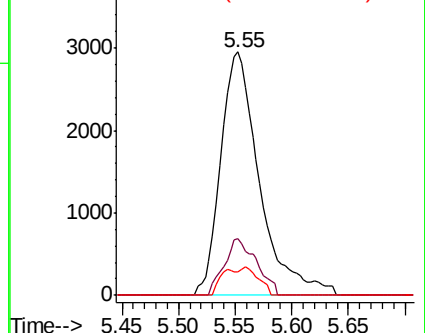

#45

1,2-Dichloropropane

Concen: 0.386 ug/l

RT: 6.70 min Scan# 1719

Delta R.T. 0.27 min

Lab File: VU029256.D


Acq: 21 Jan 2019 18:08

Tgt Ion: 63 Resp: 616

Ion Ratio Lower Upper



63 100


65 0.0 25.1 37.7#



Abundance Ion 62.90 (62.60 to 63.60): VU028994.D (-1619) (-)

Ion 64.90 (64.60 to 65.60): VU028994.D (-1619) (-)

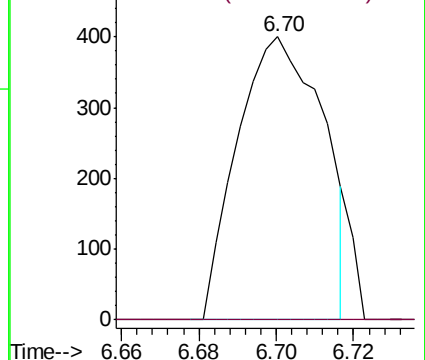



#48

Methyl methacrylate

Concen: 24.926 ug/l

RT: 6.70 min Scan# 1720

Delta R.T. 0.08 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :

CL-01-011819-A





Tgt Ion: 41 Resp: 39544

Ion Ratio Lower Upper

41 100

69 0.0 73.6 110.4#

39 46.6 39.6 59.4

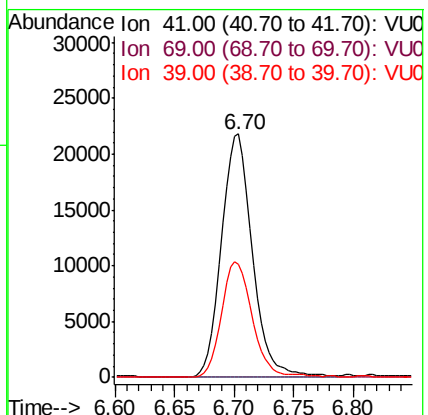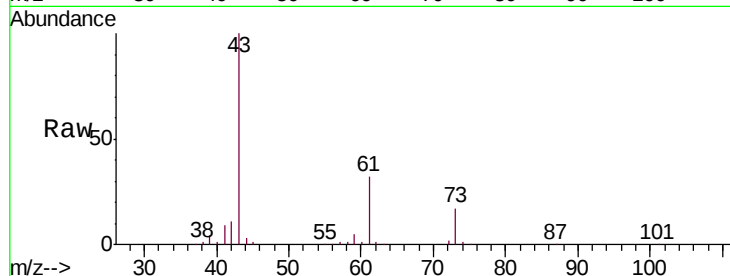

#50

Toluene-d8

Concen: 50.831 ug/l

RT: 7.56 min Scan# 1987

Delta R.T. 0.00 min

Lab File: VU029256.D




Acq: 21 Jan 2019 18:08


Tgt Ion: 98 Resp: 251822

Ion Ratio Lower Upper

98 100

100 64.2 51.6 77.4

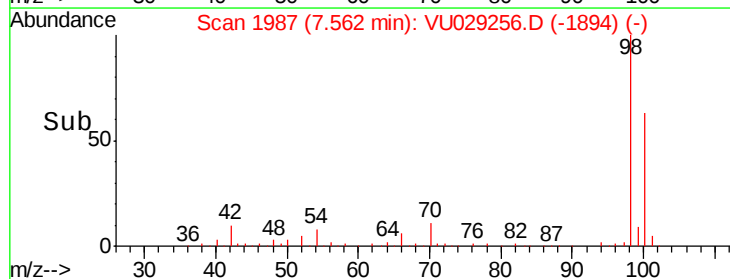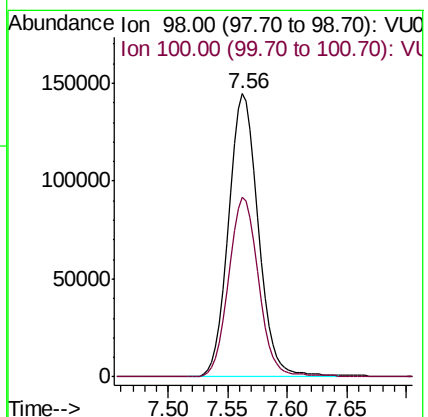

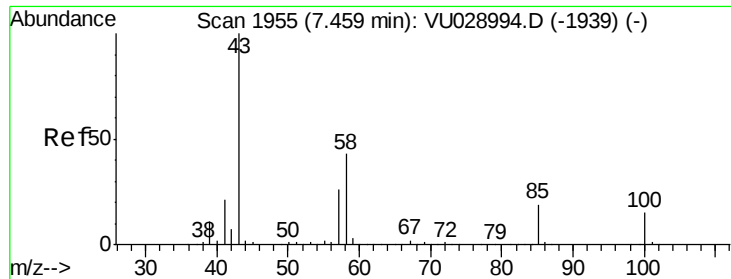

#51

4-Methyl-2-Pentanone

Concen: 16.112 ug/l

RT: 7.42 min Scan# 1942

Delta R.T. -0.04 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :


CL-01-011819-A

Tgt Ion: 43 Resp: 35727

Ion Ratio Lower Upper




43 100

58 6.3 33.9 50.9#

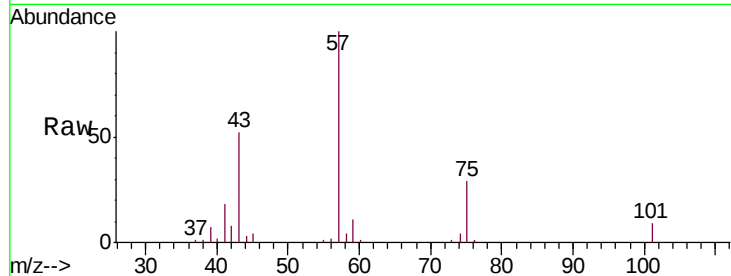

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

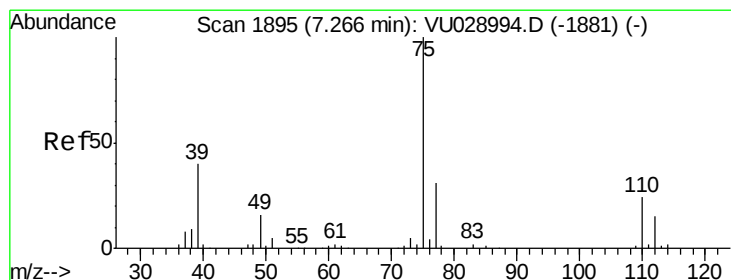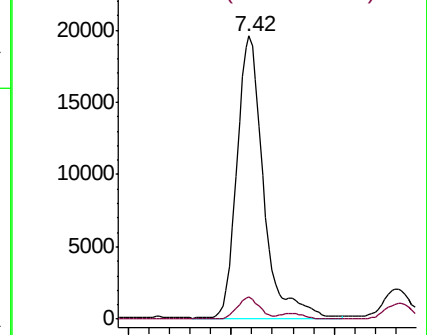

#54

cis-1,3-Dichloropropene

Concen: 7.613 ug/l

RT: 7.42 min Scan# 1942

Delta R.T. 0.15 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08


Tgt Ion: 75 Resp: 18539

Ion Ratio Lower Upper

75 100

77 0.0 25.0 37.6#



39 23.3 32.2 48.4#




Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 76.90 (76.60 to 77.60): VU0

Ion 39.00 (38.70 to 39.70): VU0




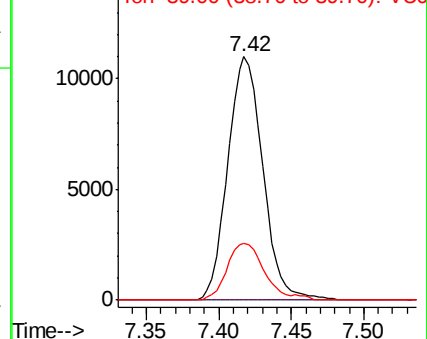




#57
 1,3-Dichloropropane
 Concen: 1.428 ug/l
 RT: 8.41 min Scan# 2252
 Delta R.T. 0.17 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08




Instrument :
 MSVOA_U
 ClientSampleId :
 CL-01-011819-A


Tgt Ion: 76 Resp: 3597
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.0 39.0#

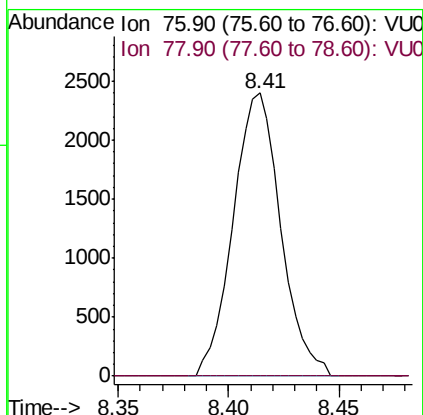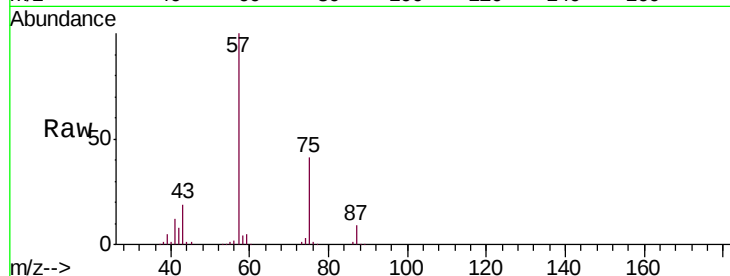

#59
 2-Hexanone
 Concen: 3.531 ug/l
 RT: 8.31 min Scan# 2219
 Delta R.T. -0.05 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08

Tgt Ion: 43 Resp: 6146
 Ion Ratio Lower Upper
 43 100
 58 0.0 29.8 89.4#

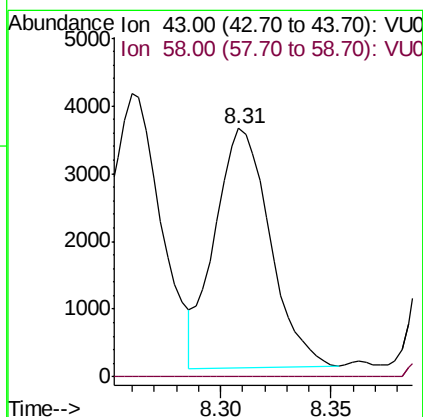



#62

4-Bromofluorobenzene

Concen: 43.683 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.00 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :

CL-01-011819-A


Tgt Ion: 95 Resp: 77774

Ion Ratio Lower Upper

95 100

174 83.2 0.0 170.6




176 80.7 0.0 165.0

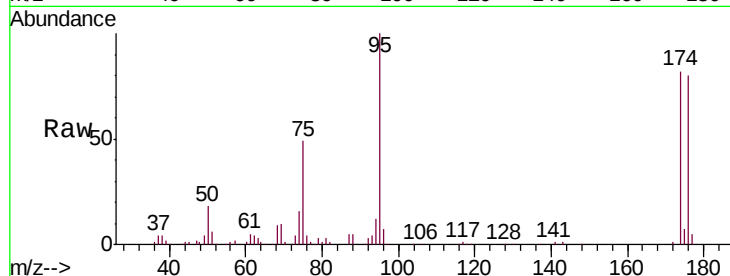

Abundance Ion 94.90 (94.60 to 95.60): VU0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

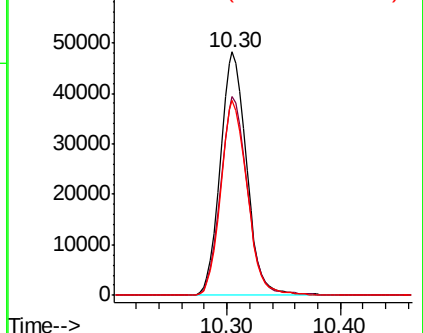

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.09 min Scan# 2461

Delta R.T. -0.00 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08


Tgt Ion: 117 Resp: 184876

Ion Ratio Lower Upper

117 100

82 55.3 43.9 65.9



119 32.2 26.0 39.0




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VU0

Ion 118.90 (118.60 to 119.60): V



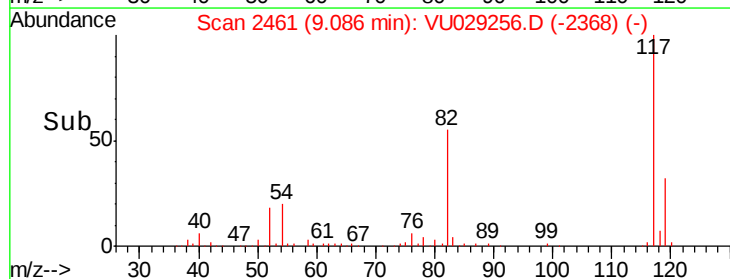
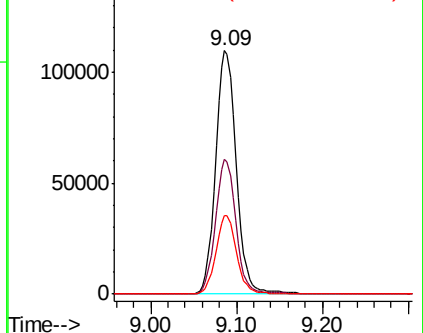


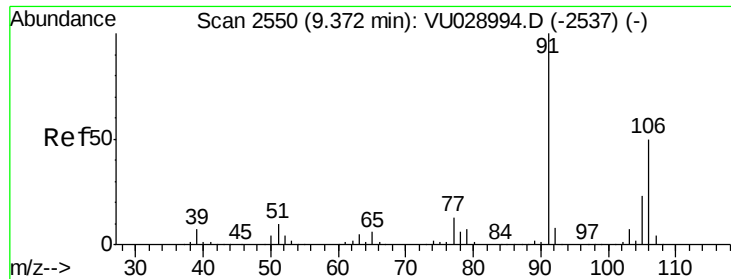

#68
m/p-Xylenes
Concen: 0.203 ug/l
RT: 9.38 min Scan# 2552
Delta R.T. 0.01 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08




Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A


Tgt Ion:106 Resp: 546
Ion Ratio Lower Upper
106 100
91 233.3 161.7 242.5

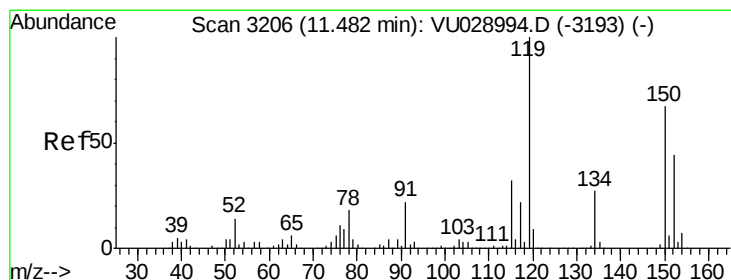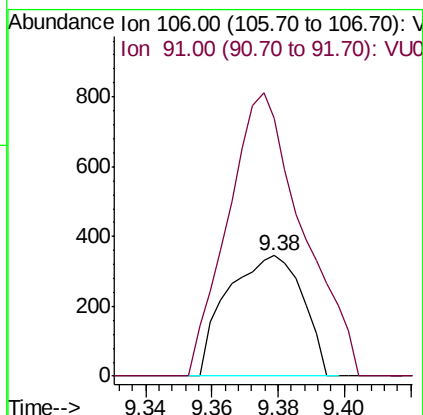

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3206
Delta R.T. -0.00 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08

Tgt Ion:152 Resp: 75598
Ion Ratio Lower Upper
152 100
115 57.9 40.1 120.3
150 155.6 0.0 345.2



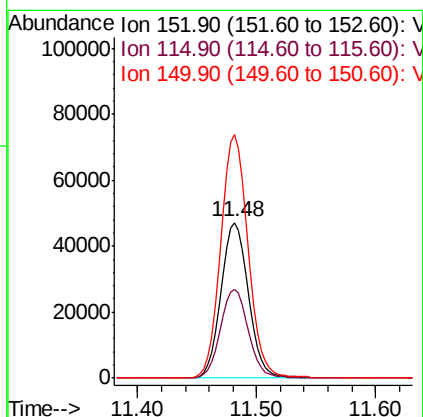
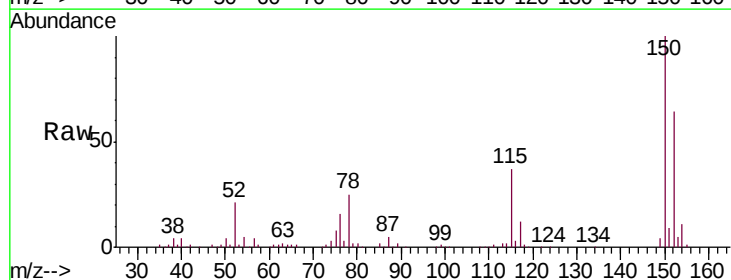


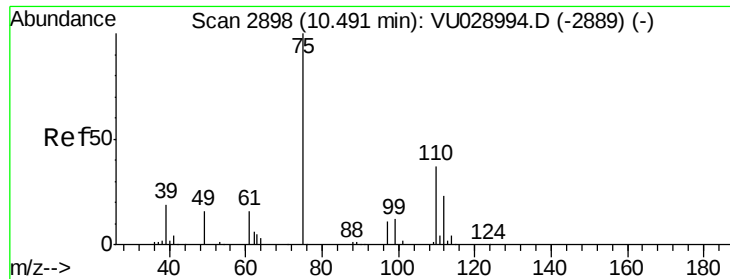

#76
 1,2,3-Trichloropropane
 Concen: 20.755 ug/l
 RT: 10.30 min Scan# 2840
 Delta R.T. -0.19 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08




Instrument :
 MSVOA_U
 ClientSampleId :
 CL-01-011819-A


Tgt Ion: 75 Resp: 38443
 Ion Ratio Lower Upper
 75 100
 77 1.0 20.9 62.8#

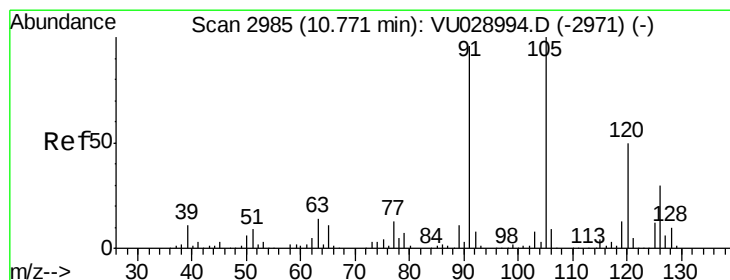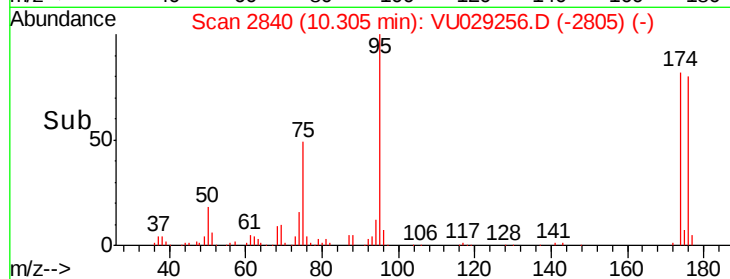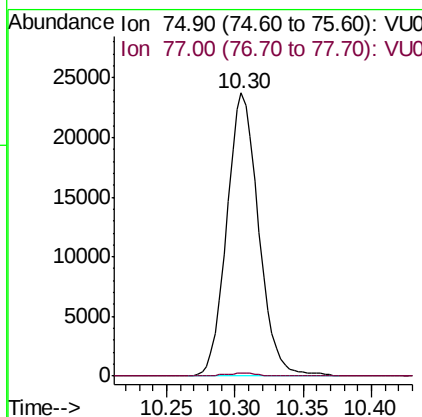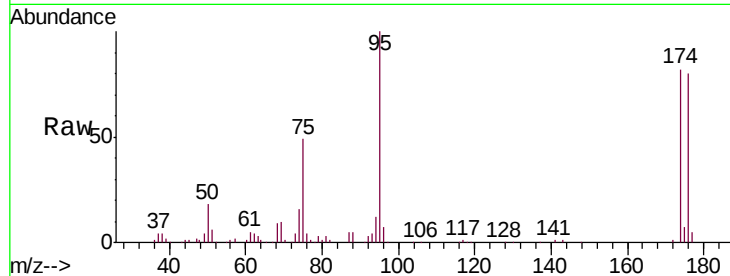

#80
 1,3,5-Trimethylbenzene
 Concen: 0.520 ug/l
 RT: 10.77 min Scan# 2985
 Delta R.T. -0.00 min
 Lab File: VU029256.D
 Acq: 21 Jan 2019 18:08

Tgt Ion: 105 Resp: 2429
 Ion Ratio Lower Upper
 105 100
 120 47.4 24.8 74.4

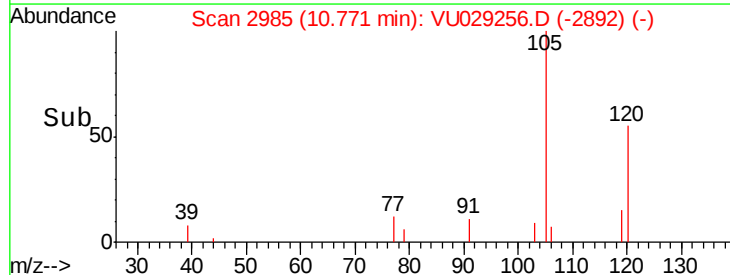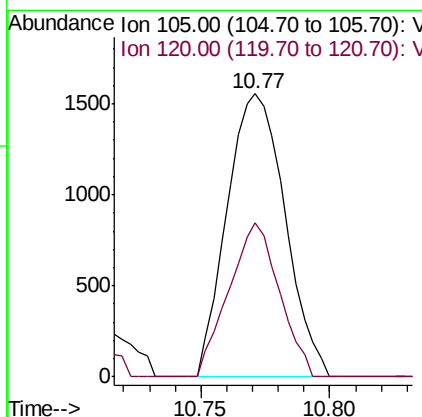



#81

trans-1,4-Dichloro-2-butene

Concen: 53.527 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.21 min

Lab File: VU029256.D

Acq: 21 Jan 2019 18:08

Instrument :

MSVOA_U

ClientSampleId :

CL-01-011819-A





Tgt Ion: 75 Resp: 38443

Ion Ratio Lower Upper

75 100

53 0.0 0.0 0.0

89 0.0 0.0 0.0

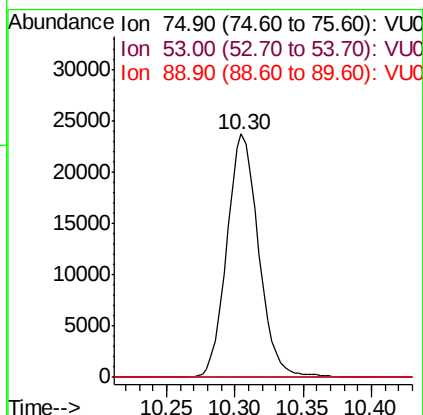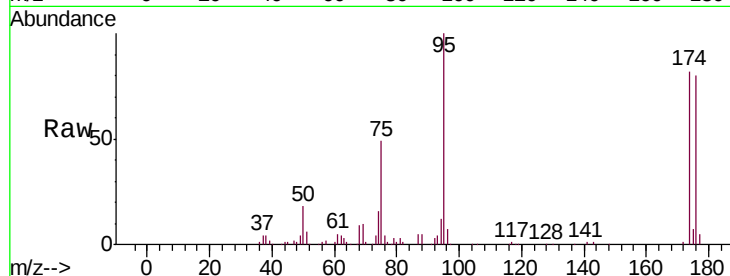

#84

1,2,4-Trimethylbenzene

Concen: 1.160 ug/l

RT: 11.15 min Scan# 3102

Delta R.T. 0.00 min

Lab File: VU029256.D




Acq: 21 Jan 2019 18:08


Tgt Ion: 105 Resp: 5411

Ion Ratio Lower Upper

105 100

120 44.8 23.1 69.3


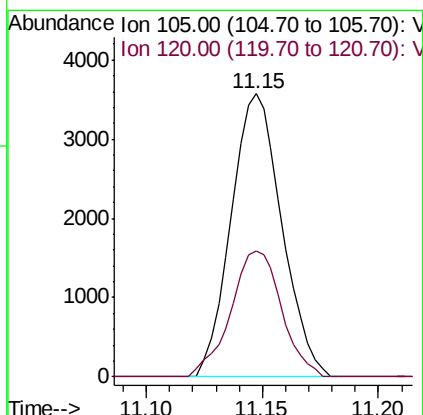




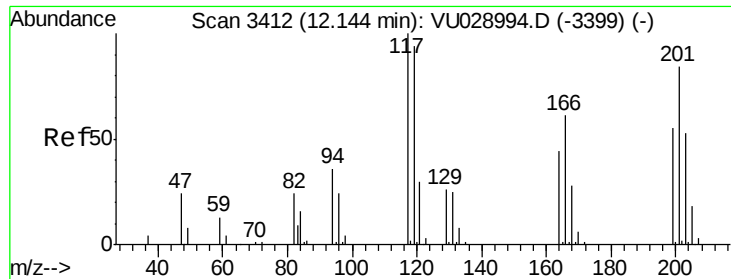

#90
Hexachloroethane
Concen: 0.348 ug/l
RT: 12.26 min Scan# 3448
Delta R.T. 0.12 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08

Instrument :
MSVOA_U
ClientSampleId :
CL-01-011819-A

Tgt Ion:117 Resp: 278
Ion Ratio Lower Upper
117 100
201 0.0 42.4 127.3#

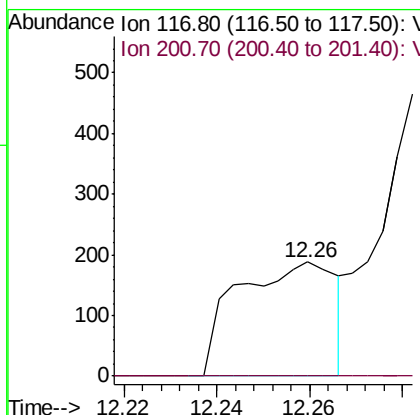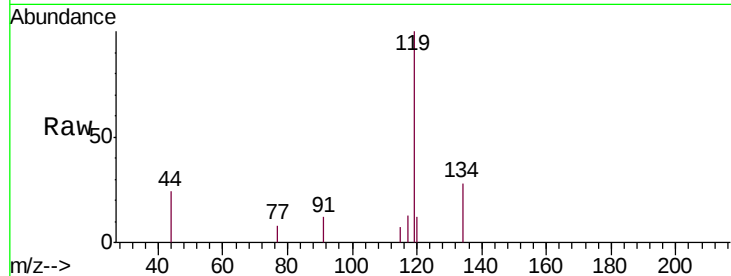

#95
Naphthalene
Concen: 5.367 ug/l
RT: 13.74 min Scan# 3909
Delta R.T. 0.00 min
Lab File: VU029256.D
Acq: 21 Jan 2019 18:08

Tgt Ion:128 Resp: 31396
Ion Ratio Lower Upper
128 100
127 13.1 10.1 15.1
129 10.3 8.5 12.7

