


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
Data File : VU042145.D
Acq On : 21 Jan 2021 12:59
Operator : SY/MD
Sample : M1170-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT95

Manual Integrations
APPROVED

SAM
1/25/2021 8:03:27 AM

Quant Time: Jan 22 02:46:52 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 22 02:43:44 2021
Response via : Initial Calibration

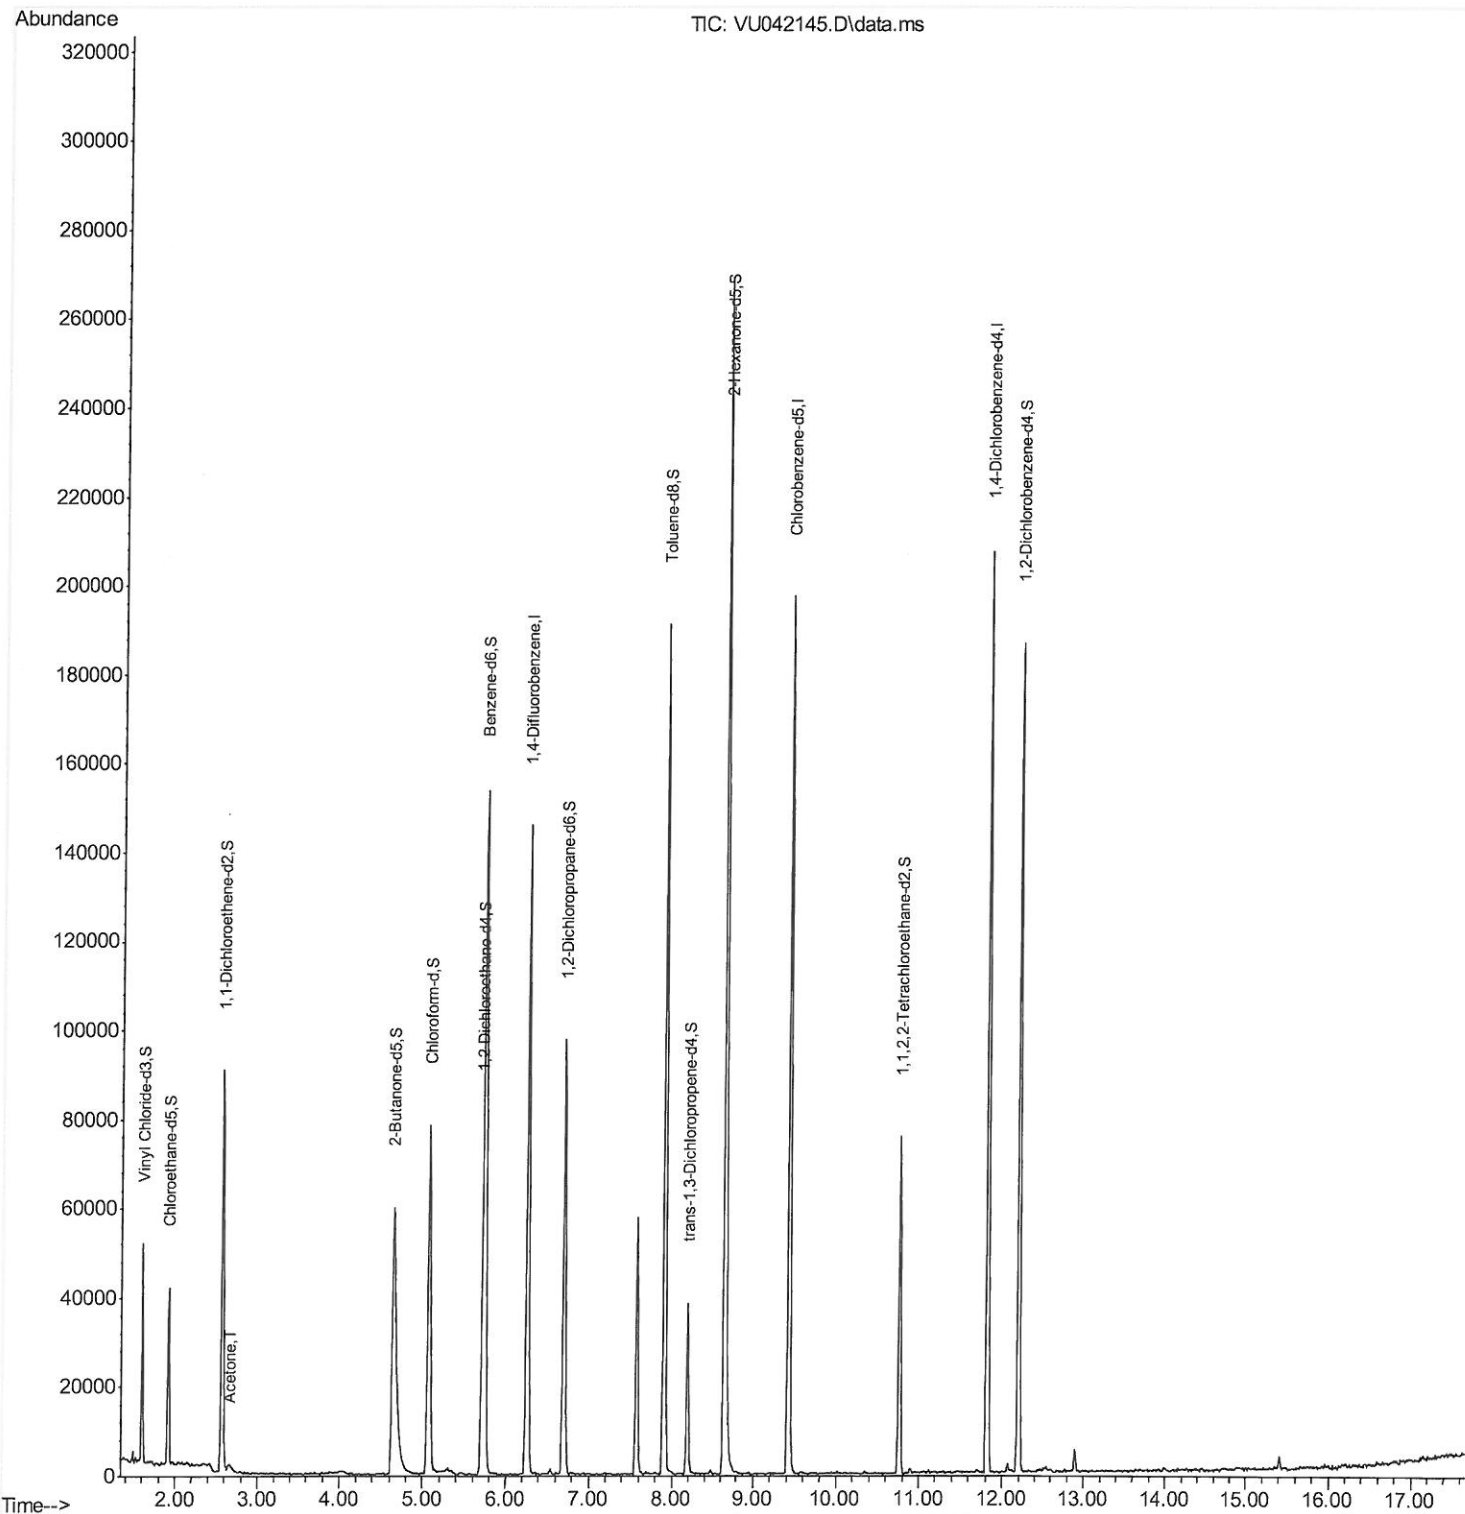

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
 Data File : VU042145.D
 Acq On : 21 Jan 2021 12:59
 Operator : SY/MD
 Sample : M1170-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT95

Manual Integrations
 APPROVED

SAM
 1/25/2021 8:03:27 AM

Quant Time: Jan 22 02:46:52 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 22 02:43:44 2021
 Response via : Initial Calibration

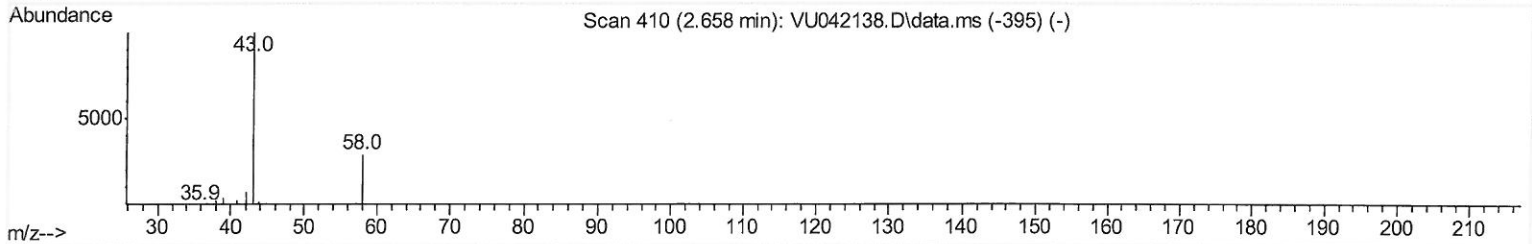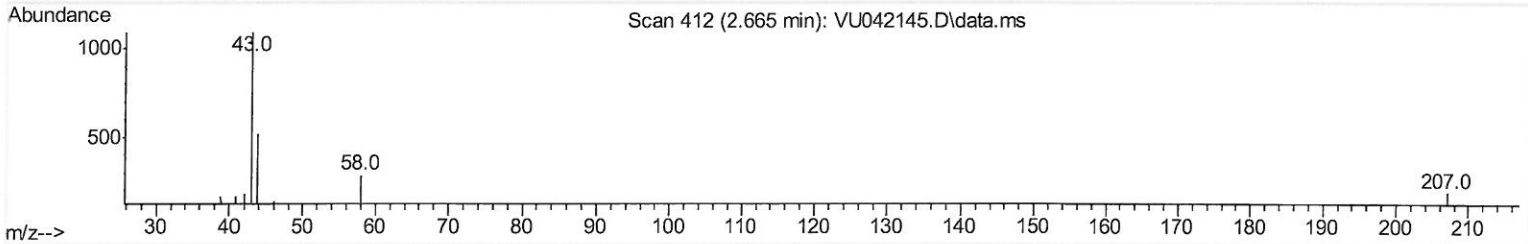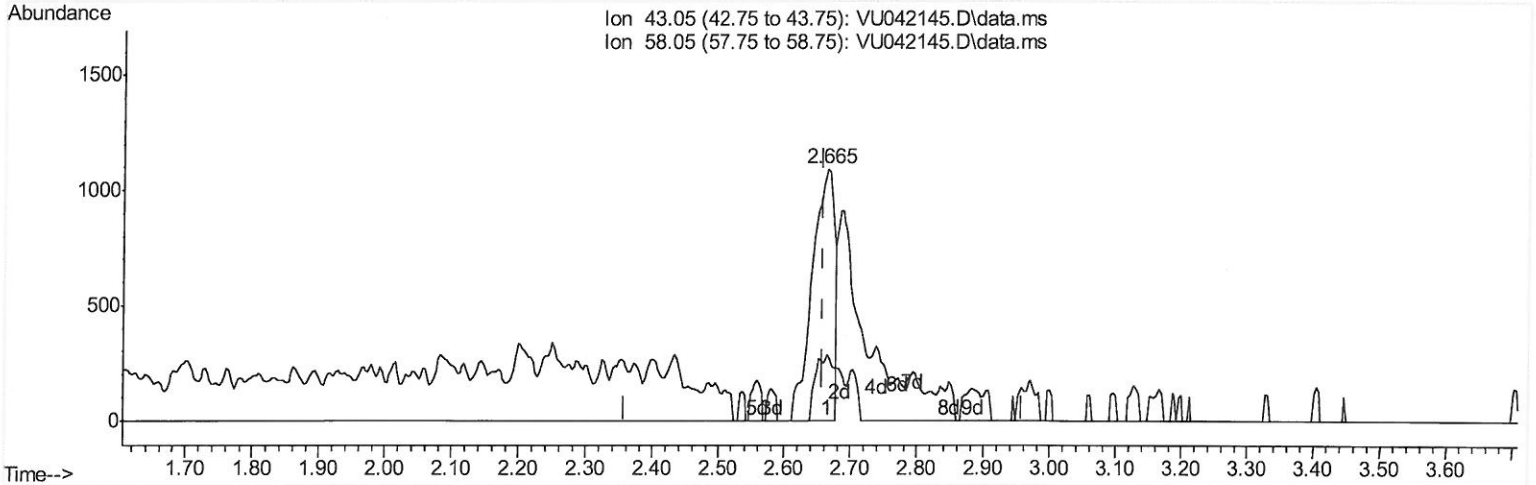

TIC: VU042145.D\data.ms

(13) Acetone (T)

2.665min (+ 0.006) 1.45 ug/L

response 2576

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.90	28.11
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
Data File : VU042145.D
Acq On : 21 Jan 2021 12:59
Operator : SY/MD
Sample : M1170-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT95

Manual Integrations
APPROVED

SAM
1/25/2021 8:03:27 AM

Quant Time: Jan 22 02:46:52 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 22 02:43:44 2021
Response via : Initial Calibration

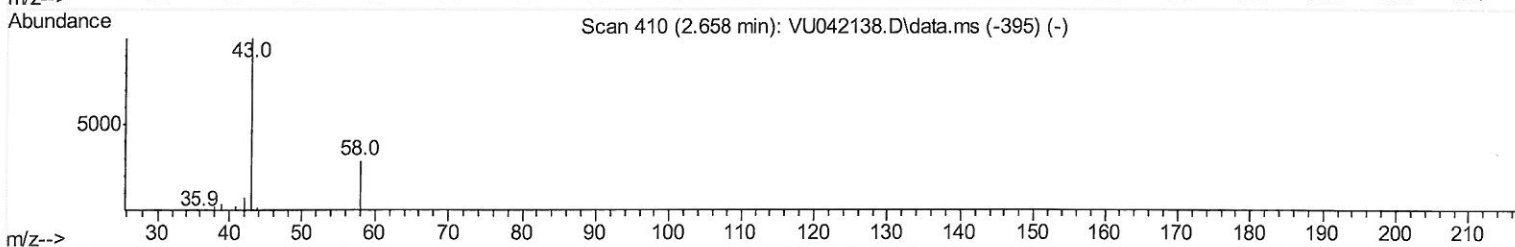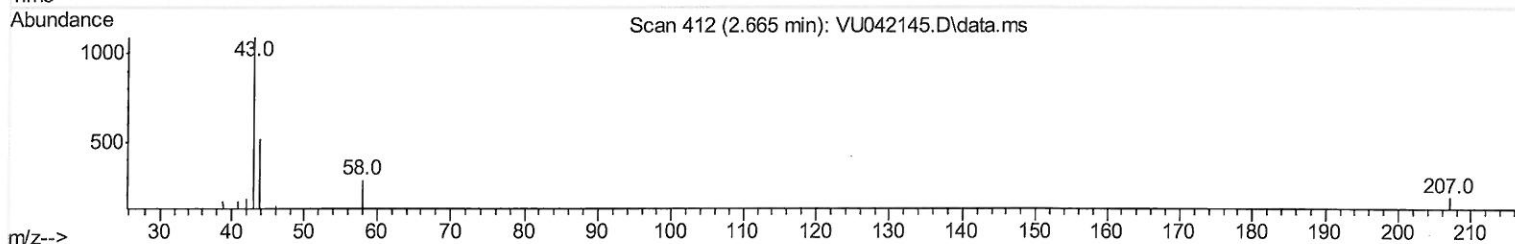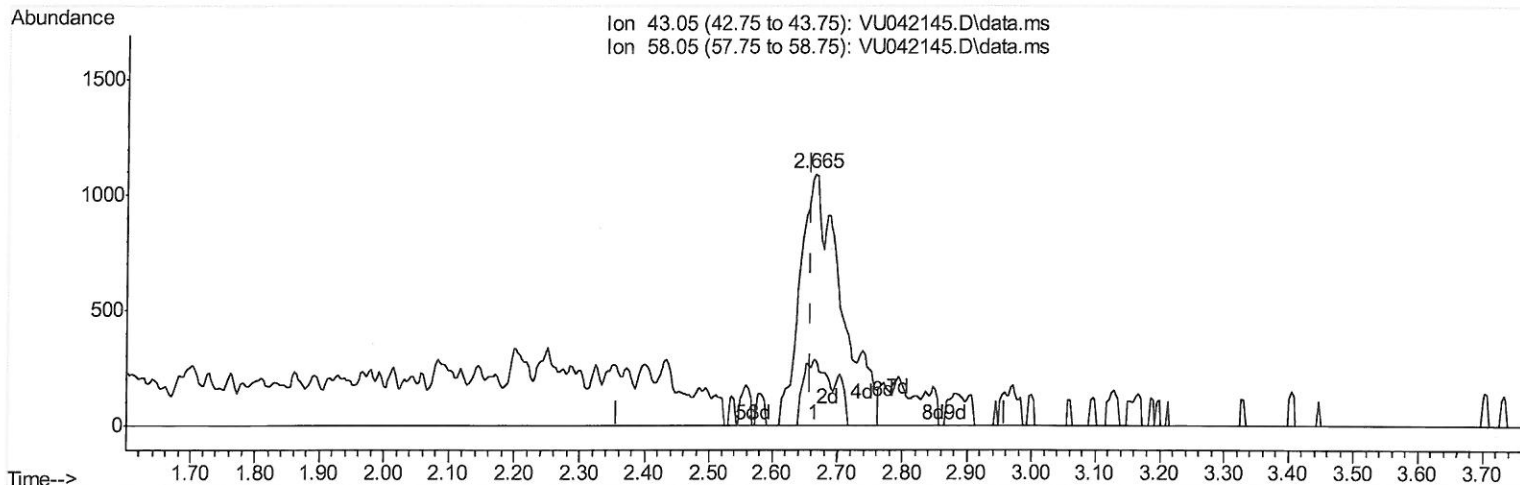

TIC: VU042145.D\data.ms

(13) Acetone (T)

2.665min (+ 0.006) 2.69 ug/L m

response 4792

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.90	15.11
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
01/25/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
 Data File : VU042145.D
 Acq On : 21 Jan 2021 12:59
 Operator : SY/MD
 Sample : M1170-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT95

Manual Integrations
 APPROVED

SAM
 1/25/2021 8:03:27 AM

Quant Time: Jan 22 02:46:52 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 22 02:43:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	113545	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	105585	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	54018	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	31770	4.34	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	86.80%		
7) Chloroethane-d5	1.919	69	26333	4.46	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	89.20%		
11) 1,1-Dichloroethene-d2	2.571	63	55429	3.43	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	68.60%		
20) 2-Butanone-d5	4.649	46	138861	51.96	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	103.92%		
24) Chloroform-d	5.073	84	70073	4.58	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.60%		
26) 1,2-Dichloroethane-d4	5.710	65	44057	4.81	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.20%		
32) Benzene-d6	5.735	84	132838	4.82	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.40%		
36) 1,2-Dichloropropane-d6	6.700	67	43333	4.87	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.40%		
41) Toluene-d8	7.906	98	119994	4.60	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	92.00%		
43) trans-1,3-Dichloroprop...	8.185	79	20207	4.48	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.60%		
46) 2-Hexanone-d5	8.645	63	98647	50.26	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	100.52%		
57) 1,1,2,2-Tetrachloroeth...	10.764	84	36017	4.72	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	94.40%		
64) 1,2-Dichlorobenzene-d4	12.201	152	47689	4.91	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	98.20%		
Target Compounds						
13) Acetone	2.665	43	4792m	2.69	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7m0
 01/25/21