

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
 Data File : VU042140.D
 Acq On : 21 Jan 2021 10:59
 Operator : SY/MD
 Sample : M1132-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK02

Quant Time: Jan 22 02:44:51 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 22 02:43:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	108475	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	100299	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	51548	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	32116	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.916	69	27738	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.40%
11) 1,1-Dichloroethene-d2	2.572	63	55684	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	4.658	46	142659	55.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.74%
24) Chloroform-d	5.073	84	72210	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.713	65	46245	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.80%
32) Benzene-d6	5.735	84	134970	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.700	67	43705	5.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.40%
41) Toluene-d8	7.906	98	123083	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
43) trans-1,3-Dichloroprop...	8.189	79	21716	5.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.40%
46) 2-Hexanone-d5	8.645	63	101760	54.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.16%
57) 1,1,2,2-Tetrachloroeth...	10.767	84	38254	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	48884	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%
Target Compounds						Qvalue
16) Methylene chloride	3.051	84	3155	0.36	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
Data File : VU042140.D
Acq On : 21 Jan 2021 10:59
Operator : SY/MD
Sample : M1132-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02


Quant Time: Jan 22 02:44:51 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 22 02:43:44 2021
Response via : Initial Calibration

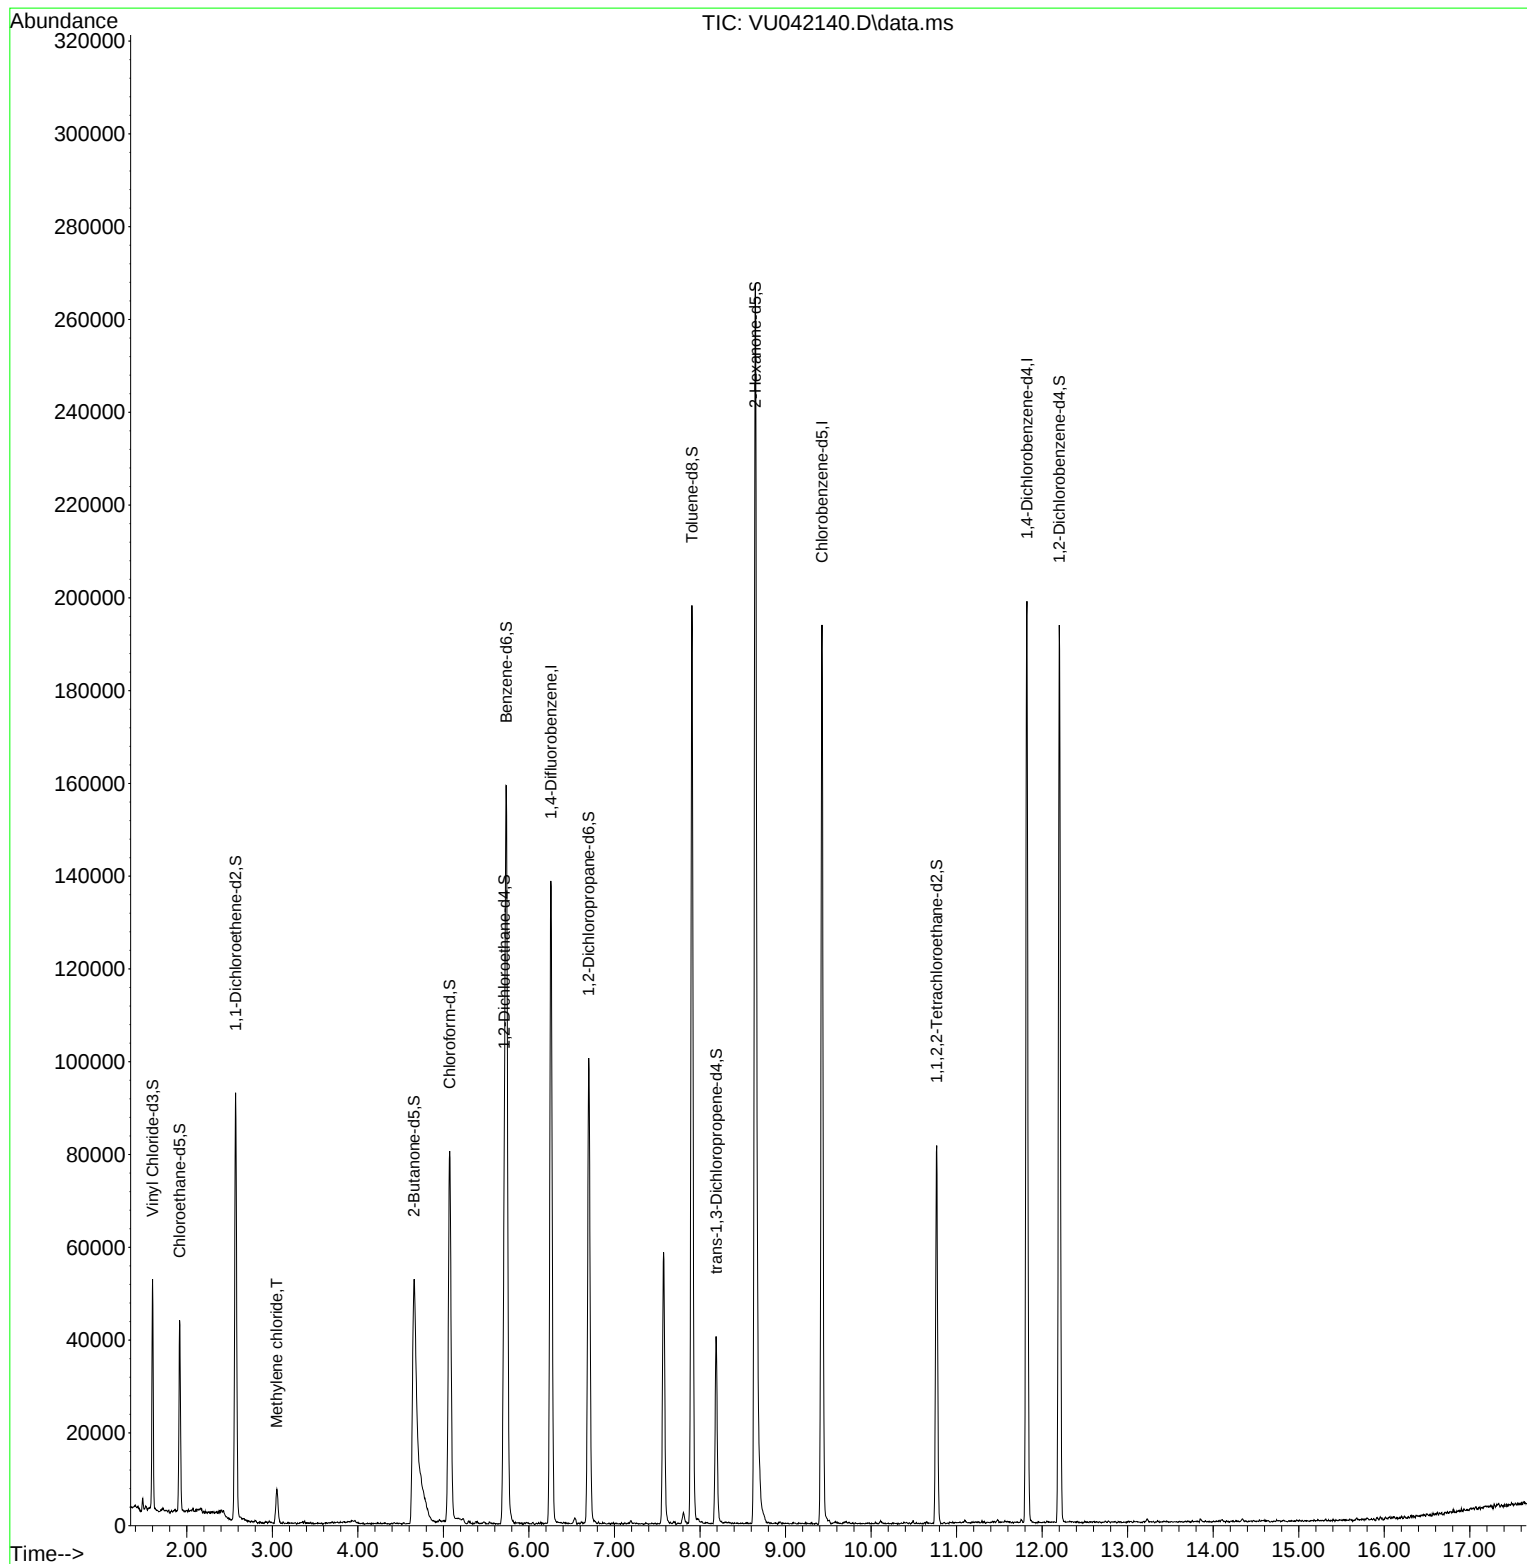

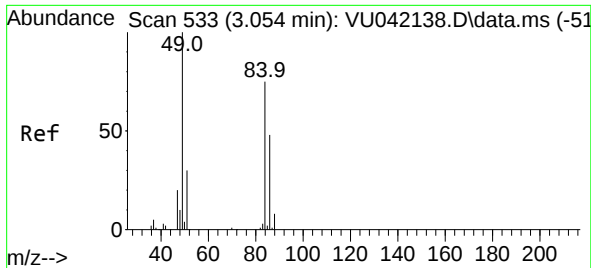

#16
Methylene chloride
Concen: 0.36 ug/L
RT: 3.051 min Scan# 532
Delta R.T. -0.003 min
Lab File: VU042140.D
Acq: 21 Jan 2021 10:59

Instrument :
MSVOA_U
ClientSampleId :
VHBLK02

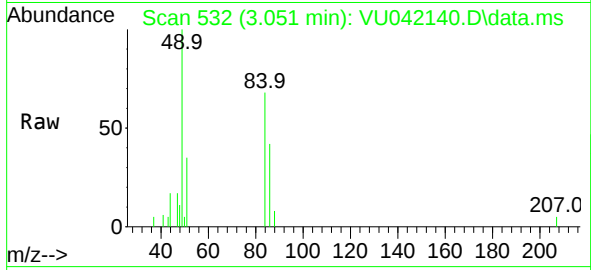

Tgt Ion:	84	Resp:	3155
Ion	Ratio	Lower	Upper
84	100		
86	62.1	44.1	81.9
49	147.0	95.0	176.4

