

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
 Data File : VU042146.D
 Acq On : 21 Jan 2021 13:23
 Operator : SY/MD
 Sample : M1170-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT96

Quant Time: Jan 22 02:47:09 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 22 02:43:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	110028	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	102082	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	52491	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	33854	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.916	69	27843	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.572	63	57075	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	4.646	46	142803	55.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.28%
24) Chloroform-d	5.073	84	72672	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.710	65	45736	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.736	84	137322	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.700	67	45671	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.906	98	125511	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
43) trans-1,3-Dichloroprop...	8.189	79	21339	4.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.00%
46) 2-Hexanone-d5	8.642	63	102090	53.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.60%
57) 1,1,2,2-Tetrachloroeth...	10.765	84	37807	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.60%
64) 1,2-Dichlorobenzene-d4	12.202	152	49351	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%
Target Compounds					Qvalue	
13) Acetone	2.659	43	2357	1.37	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
Data File : VU042146.D
Acq On : 21 Jan 2021 13:23
Operator : SY/MD
Sample : M1170-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT96


Quant Time: Jan 22 02:47:09 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 22 02:43:44 2021
Response via : Initial Calibration

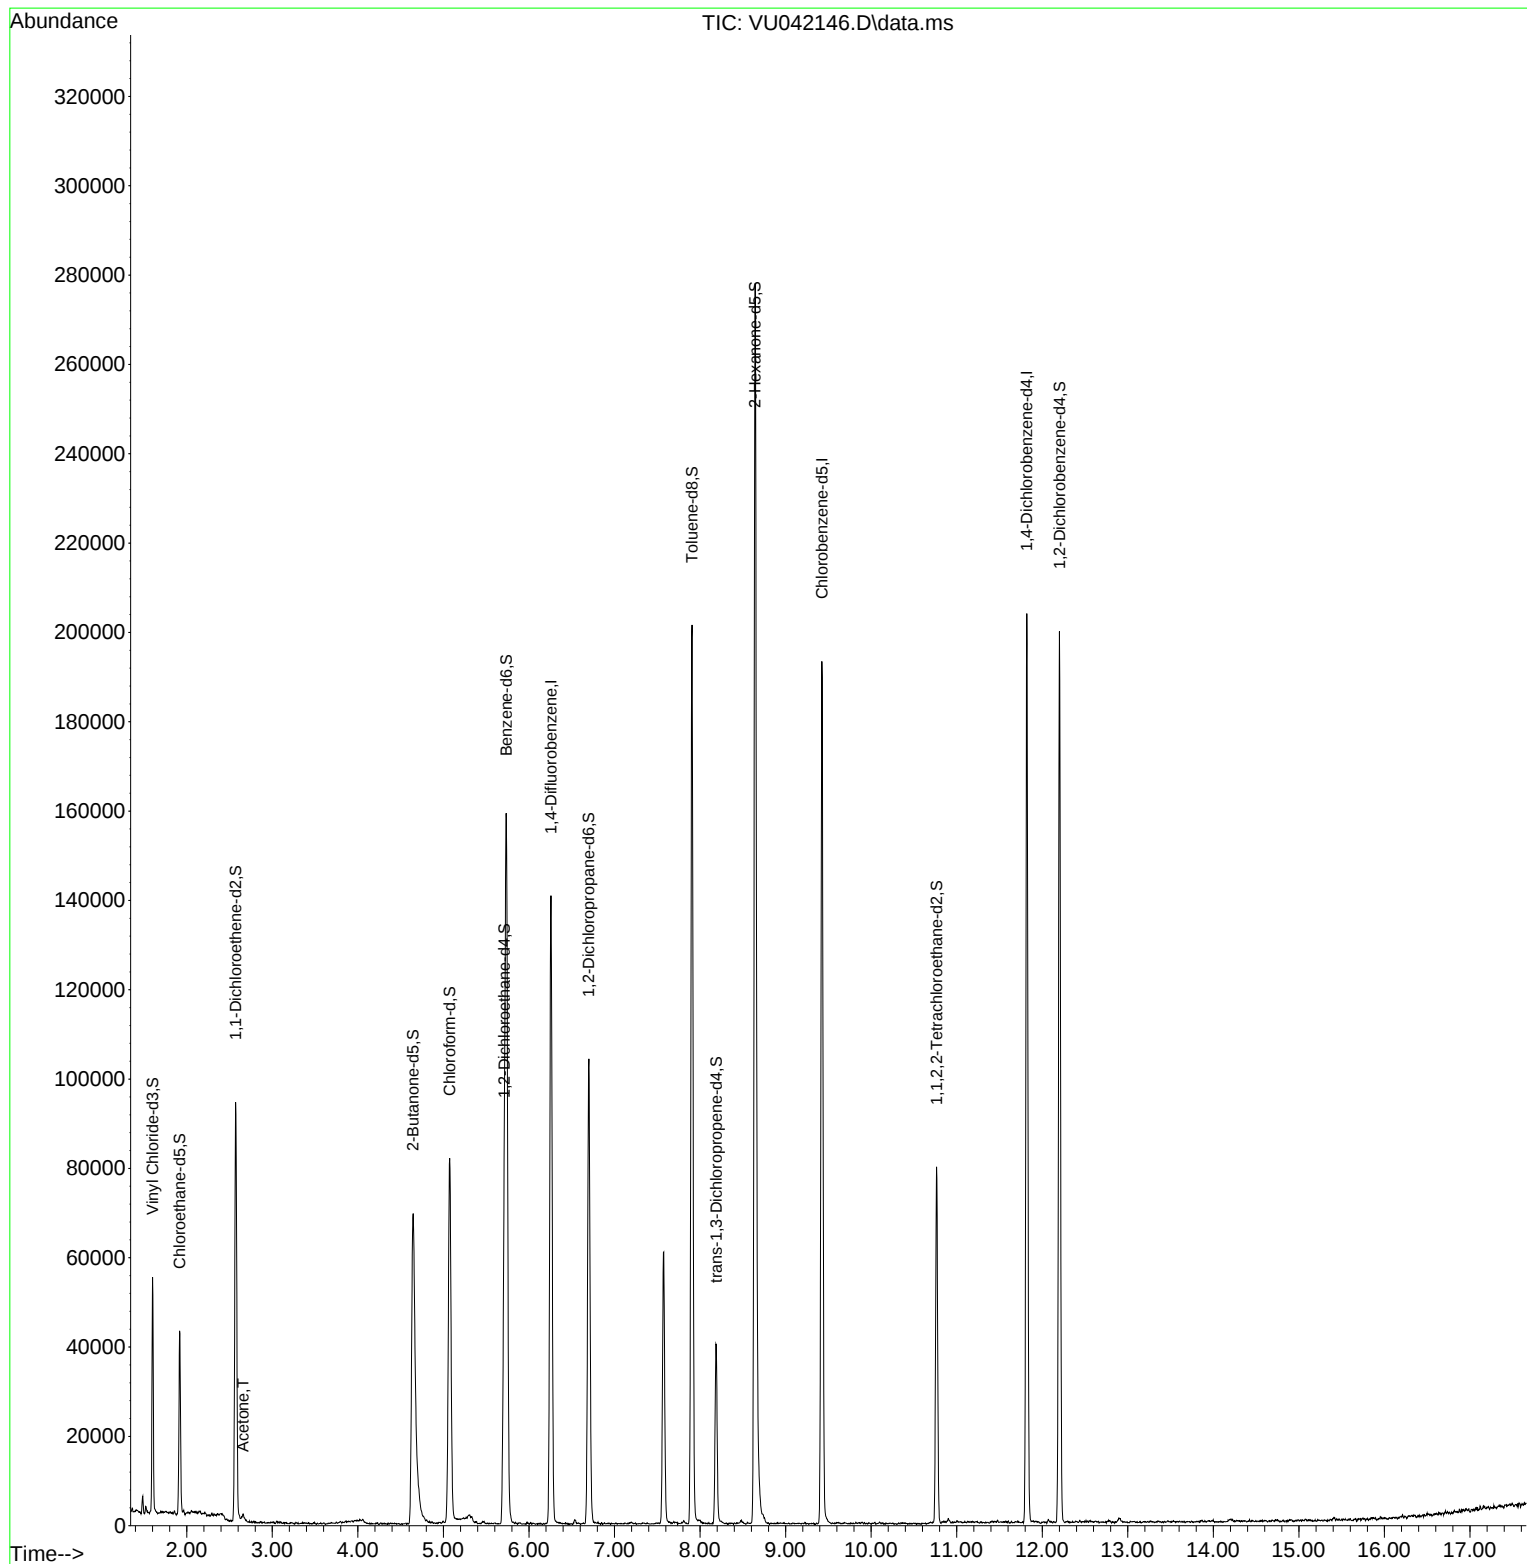

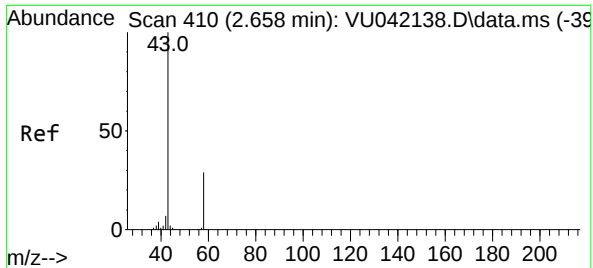

#13
 Acetone
 Concen: 1.37 ug/L
 RT: 2.659 min Scan# 410
 Delta R.T. 0.000 min
 Lab File: VU042146.D
 Acq: 21 Jan 2021 13:23

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT96

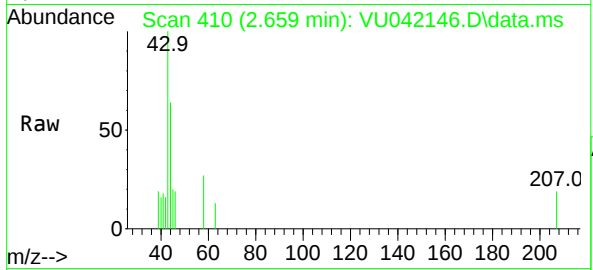

Tgt Ion: 43 Resp: 2357
 Ion Ratio Lower Upper
 43 100
 58 18.0 0.0 55.8

