
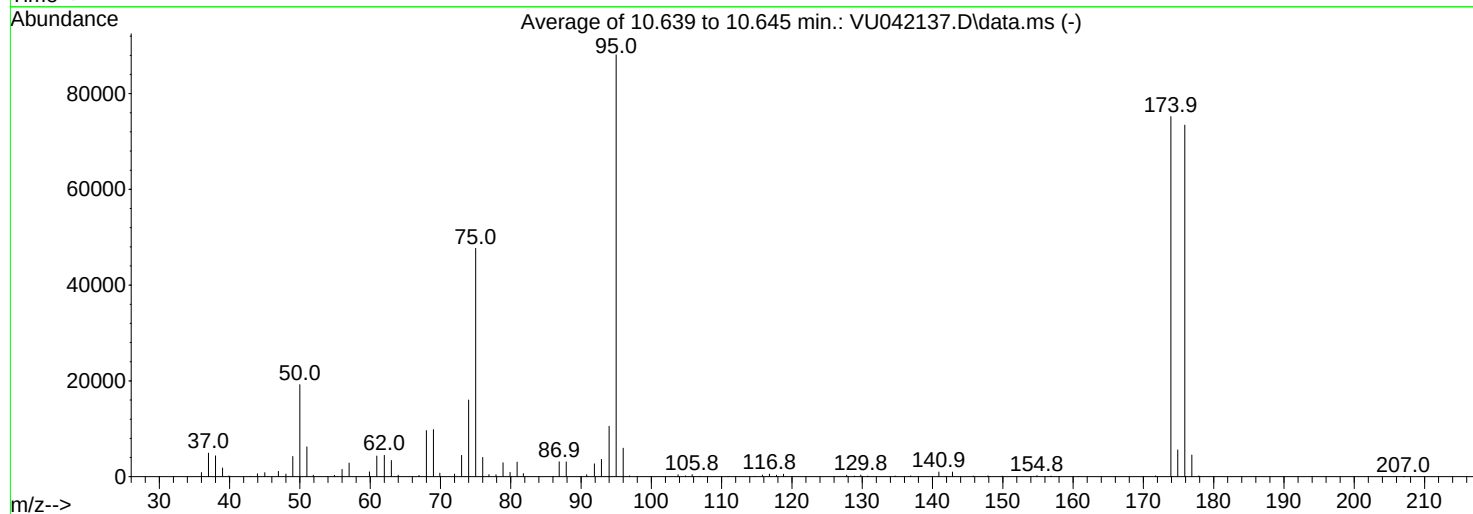


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012121\
Data File : VU042137.D
Acq On : 21 Jan 2021 09:05
Operator : SY/MD
Sample : BFB39
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jan 23 06:18:59 2021

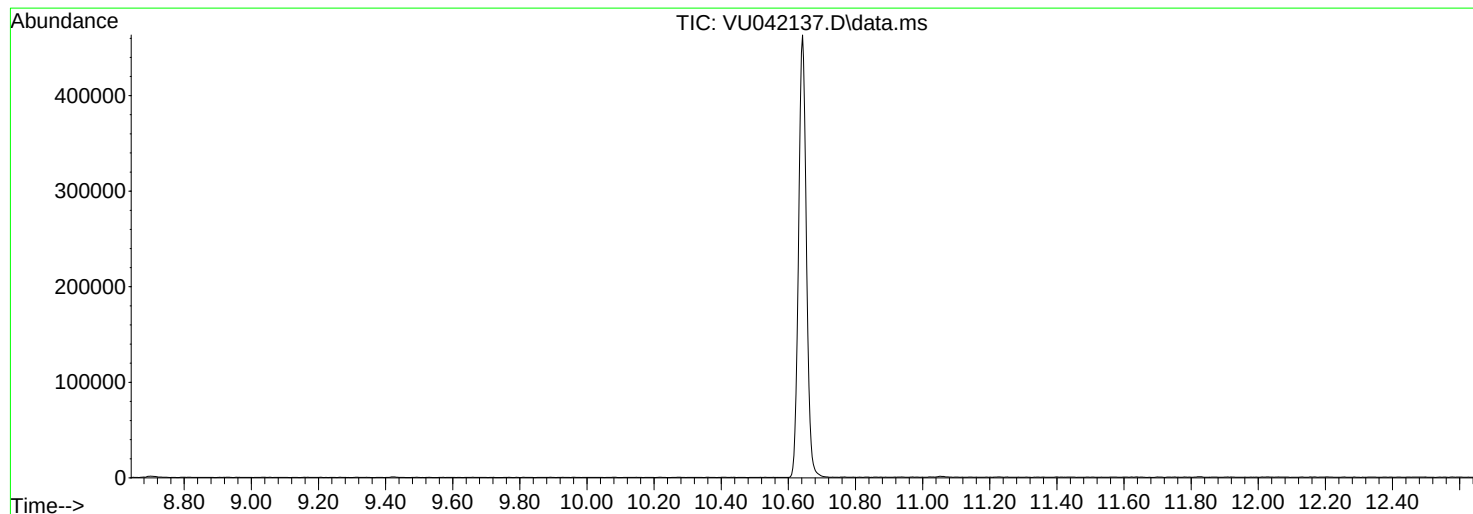

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	19235	PASS
75	95	30	80	54.1	47683	PASS
95	95	100	100	100.0	88091	PASS
96	95	5	9	6.7	5939	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.4	75205	PASS
175	174	5	9	7.4	5584	PASS
176	174	95	101	97.6	73416	PASS
177	176	5	9	6.1	4499	PASS

m/z	Abundance
43.90	358.0
207.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	969.0
37.00	4963.0
38.00	4463.0
39.00	1873.0
39.90	178.0
42.90	100.0
44.00	989.0
45.00	873.0
47.00	1053.0
48.00	515.0
49.00	4197.0
50.00	19424.0
51.00	6153.0
51.90	301.0
54.90	267.0
56.00	1467.0
57.00	2841.0
59.90	950.0
61.00	4356.0
62.00	4520.0
63.00	3535.0
64.00	338.0
66.90	297.0
68.00	9585.0
69.00	9862.0
69.90	771.0
72.00	533.0
73.00	4464.0
74.00	16215.0
75.00	47680.0
76.00	4085.0
76.90	457.0
77.90	437.0
78.90	2822.0
79.90	896.0
80.90	3099.0
81.80	603.0
86.90	3047.0
87.90	3056.0
90.80	410.0
91.90	2777.0
92.90	3661.0
94.00	10600.0
95.00	87696.0
96.00	6210.0
96.90	168.0
103.80	441.0
104.90	155.0
105.80	426.0
106.90	102.0
114.80	101.0
115.80	355.0
116.80	520.0
117.80	311.0
118.80	449.0
127.80	264.0
128.90	140.0
129.80	322.0
130.80	118.0
134.70	131.0
136.90	184.0
140.90	888.0
141.80	107.0
142.80	999.0
145.80	122.0
147.90	173.0
149.90	119.0
154.90	209.0
156.90	127.0
160.80	112.0
171.80	165.0
173.90	72952.0
174.90	5577.0
175.90	70952.0
176.90	4455.0
177.90	150.0
207.00	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	869.0
37.00	5011.0
38.00	4475.0
39.00	1862.0
39.90	189.0
43.00	120.0
44.00	974.0
45.00	887.0
46.90	1150.0
48.00	542.0
49.00	4368.0
50.00	19848.0
51.00	6451.0
51.90	322.0
54.90	289.0
56.00	1603.0
57.00	2939.0
59.90	1058.0
61.00	4482.0
62.00	4587.0
63.00	3511.0
64.00	313.0
66.90	288.0
68.00	9986.0
69.00	10064.0
69.90	782.0
72.00	556.0
73.00	4658.0
74.00	16512.0
75.00	49288.0
76.00	4120.0
76.90	424.0
77.90	446.0
78.90	2968.0
79.90	936.0
80.90	3133.0
81.80	656.0
86.90	3188.0
87.90	3183.0
90.80	414.0
91.90	2743.0
92.90	3703.0
94.00	10702.0
95.00	90760.0
96.00	6134.0
96.90	155.0
103.80	429.0
104.80	165.0
105.80	432.0
106.90	106.0
110.90	111.0
114.70	102.0
115.80	365.0
116.80	548.0
117.80	283.0
118.80	505.0
127.80	298.0
128.90	149.0
129.80	354.0
130.80	158.0
134.70	158.0
136.90	187.0
140.90	1009.0
141.80	112.0
142.90	996.0
145.80	121.0
147.90	187.0
149.90	112.0
154.80	227.0
156.80	127.0
171.70	169.0
173.90	77840.0
174.90	5736.0
175.90	75816.0
176.90	4617.0
177.90	169.0
207.00	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
36.00	745.0
37.00	4753.0
38.00	4078.0
39.00	1698.0
39.90	170.0
44.00	894.0
45.00	788.0
46.90	1087.0
48.00	505.0
49.00	4073.0
50.00	18432.0
51.00	6021.0
51.90	266.0
54.90	249.0
56.00	1488.0
57.00	2748.0
59.90	967.0
60.90	4118.0
62.00	4251.0
63.00	3130.0
64.00	253.0
67.00	247.0
68.00	9272.0
69.00	9523.0
69.90	708.0
72.00	540.0
73.00	4195.0
74.00	15249.0
75.00	46080.0
76.00	3870.0
76.90	399.0
77.90	374.0
78.90	2915.0
79.90	895.0
80.90	2905.0
81.80	639.0
86.00	102.0
86.90	3143.0
87.90	3044.0
90.80	367.0
91.90	2513.0
92.90	3474.0
94.00	10235.0
95.00	85816.0
96.00	5472.0
96.90	136.0
103.80	384.0
104.80	169.0
105.80	403.0
110.90	104.0
115.80	317.0
116.80	532.0
117.80	273.0
118.80	543.0
127.80	302.0
128.90	154.0
129.80	320.0
130.80	166.0
134.70	164.0
136.90	181.0
140.90	1033.0
142.90	922.0
145.80	120.0
147.90	180.0
149.90	104.0
154.80	236.0
156.80	120.0
171.80	160.0
173.90	74824.0
174.90	5440.0
175.90	73480.0
176.90	4426.0
177.90	144.0
207.00	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39