


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012122\
 Data File : VU046818.D
 Acq On : 21 Jan 2022 09:05
 Operator : SY/MD
 Sample : BFB046
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB046

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jan 24 00:23:26 2022

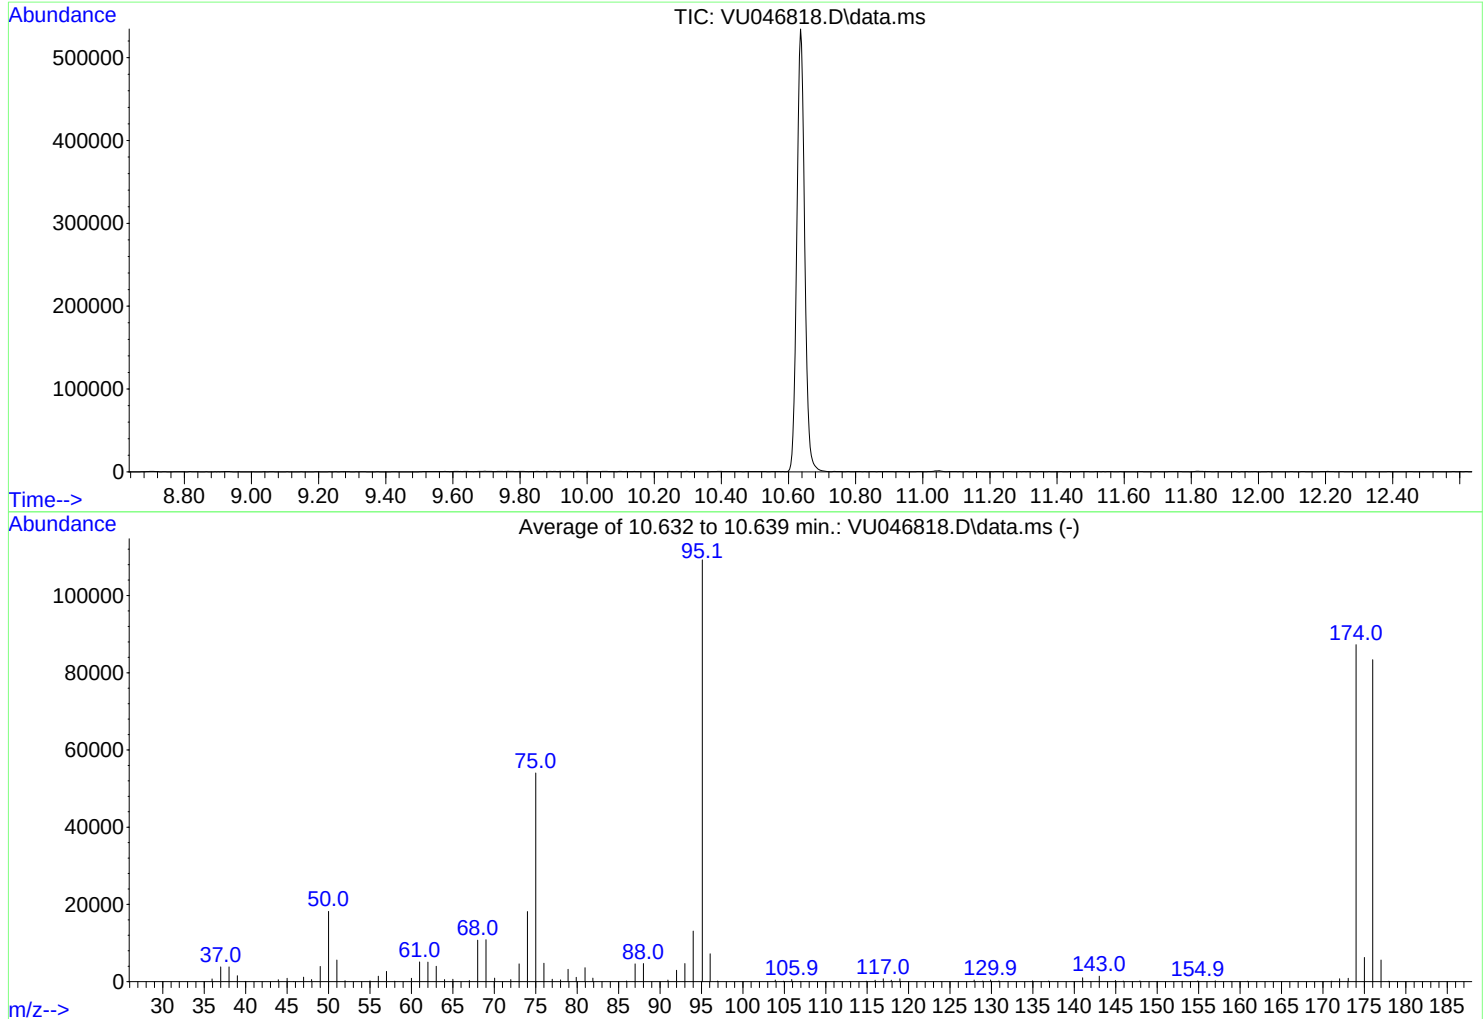

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	18197	PASS
75	95	30	80	49.5	54040	PASS
95	95	100	100	100.0	109248	PASS
96	95	5	9	6.6	7206	PASS
173	174	0.00	2	1.0	865	PASS
174	95	50	120	79.9	87288	PASS
175	174	5	9	7.2	6271	PASS
176	174	95	101	95.5	83403	PASS
177	176	5	9	6.7	5596	PASS

Scan 2876 (10.587 min): VU046818.D\data.ms
BFB046

m/z	Abundance
35.80	193.0
43.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	844.0
37.00	3689.0
38.00	3719.0
39.00	1484.0
39.90	121.0
44.00	622.0
45.00	890.0
45.80	109.0
47.00	1105.0
47.90	575.0
49.00	3897.0
50.00	17928.0
51.00	5559.0
52.00	239.0
55.00	174.0
56.00	1332.0
57.00	2708.0
58.00	156.0
60.00	872.0
61.00	4915.0
62.00	5177.0
63.00	3874.0
64.00	514.0
65.00	668.0
67.00	275.0
68.00	10413.0
69.00	10425.0
70.00	908.0
72.00	508.0
73.00	4410.0
74.00	17664.0
75.00	52888.0
76.00	4745.0
77.00	575.0
78.00	431.0
78.90	3169.0
79.90	1034.0
80.90	3444.0
81.90	820.0
85.90	151.0
87.00	4413.0
88.00	4366.0
91.00	403.0
92.00	2843.0
93.00	4539.0
94.00	12560.0
95.10	107112.0
96.10	7145.0
97.00	156.0
103.90	414.0
104.90	130.0
105.90	512.0
106.90	119.0
111.00	103.0
112.90	119.0
114.90	113.0
115.90	350.0
117.00	730.0
117.90	385.0
118.90	754.0
127.90	357.0
128.90	166.0
129.90	424.0
130.90	189.0
135.00	163.0
136.90	159.0
141.00	907.0
141.90	101.0
143.00	1461.0
145.00	282.0
145.90	187.0
147.90	205.0
150.00	105.0
153.00	101.0
154.90	198.0
157.00	188.0
158.90	132.0
160.90	113.0
171.10	105.0
172.00	814.0
173.10	798.0
174.00	83064.0
175.00	6175.0
176.00	79080.0
177.00	5379.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	908.0
37.00	3888.0
38.00	3907.0
39.00	1581.0
40.00	101.0
44.00	650.0
45.00	916.0
47.00	1198.0
47.90	565.0
49.00	4087.0
50.00	18728.0
51.00	5820.0
52.00	242.0
55.00	201.0
56.00	1454.0
57.00	2729.0
58.00	123.0
60.00	916.0
61.00	5248.0
62.00	5262.0
63.00	4125.0
64.00	566.0
65.00	655.0
67.00	279.0
68.00	11128.0
69.00	11270.0
70.00	947.0
72.00	535.0
73.00	4784.0
74.00	18744.0
75.00	55816.0
76.00	4967.0
77.00	624.0
78.00	491.0
78.90	3245.0
79.90	1134.0
80.90	3789.0
81.90	933.0
85.90	158.0
87.00	4767.0
88.00	4879.0
91.00	419.0
92.00	3022.0
93.00	4882.0
94.00	13528.0
95.10	112560.0
96.00	7411.0
96.90	150.0
103.90	439.0
104.90	140.0
105.90	538.0
106.90	108.0
111.00	113.0
112.90	120.0
114.90	134.0
116.00	392.0
117.00	755.0
117.90	398.0
118.90	789.0
127.90	404.0
129.00	181.0
129.90	451.0
130.90	213.0
135.00	190.0
136.90	187.0
141.00	997.0
143.00	1489.0
145.00	299.0
145.90	169.0
147.90	229.0
150.00	114.0
153.00	112.0
154.90	198.0
157.00	192.0
158.90	109.0
160.90	128.0
171.00	125.0
172.00	782.0
173.00	879.0
174.00	90408.0
175.00	6497.0
176.00	85976.0
177.00	5785.0
178.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
36.00	890.0
37.00	3844.0
38.00	3776.0
39.00	1579.0
44.00	586.0
45.00	824.0
47.00	1181.0
48.00	508.0
49.00	3777.0
50.00	17936.0
51.00	5443.0
52.00	221.0
55.00	212.0
56.00	1442.0
57.00	2559.0
58.00	114.0
60.00	848.0
61.00	5128.0
62.00	4749.0
63.00	3911.0
64.00	549.0
65.00	565.0
67.00	292.0
68.00	10684.0
69.00	10824.0
70.10	860.0
72.00	549.0
73.00	4672.0
74.00	18040.0
75.00	53416.0
76.00	4594.0
77.00	646.0
78.00	491.0
78.90	3157.0
79.90	1139.0
81.00	3644.0
81.90	944.0
86.00	139.0
87.00	4625.0
88.00	4749.0
90.90	382.0
92.00	2953.0
93.00	4627.0
94.00	13225.0
95.10	108072.0
96.00	7062.0
96.90	146.0
103.90	435.0
104.90	145.0
105.90	516.0
114.90	131.0
116.00	394.0
116.90	765.0
117.90	389.0
119.00	703.0
123.90	107.0
127.90	434.0
129.00	198.0
129.90	438.0
130.90	193.0
134.90	215.0
136.90	188.0
141.00	1032.0
143.00	1336.0
144.90	288.0
145.90	145.0
147.90	231.0
154.90	214.0
157.00	185.0
160.90	124.0
171.00	118.0
172.00	701.0
173.00	918.0
174.00	88392.0
175.00	6142.0
176.00	85152.0
177.00	5624.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046