
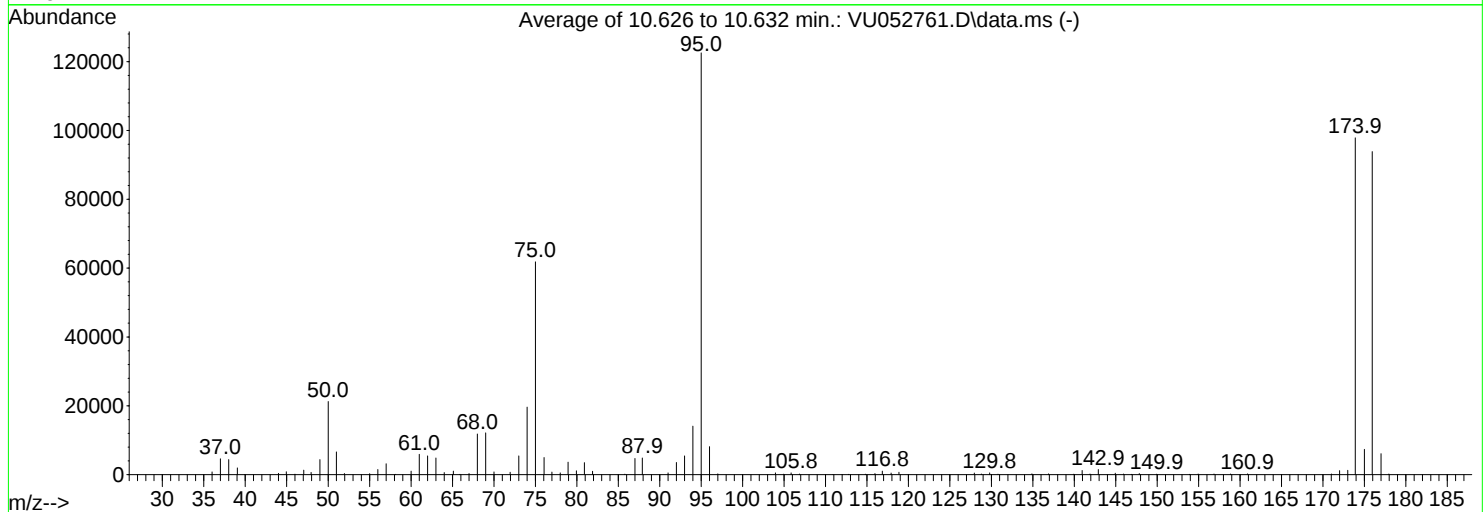


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012123\
Data File : VU052761.D
Acq On : 20 Jan 2023 14:50
Operator : JC/MD
Sample : BFB192
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB192

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jan 21 01:44:26 2023

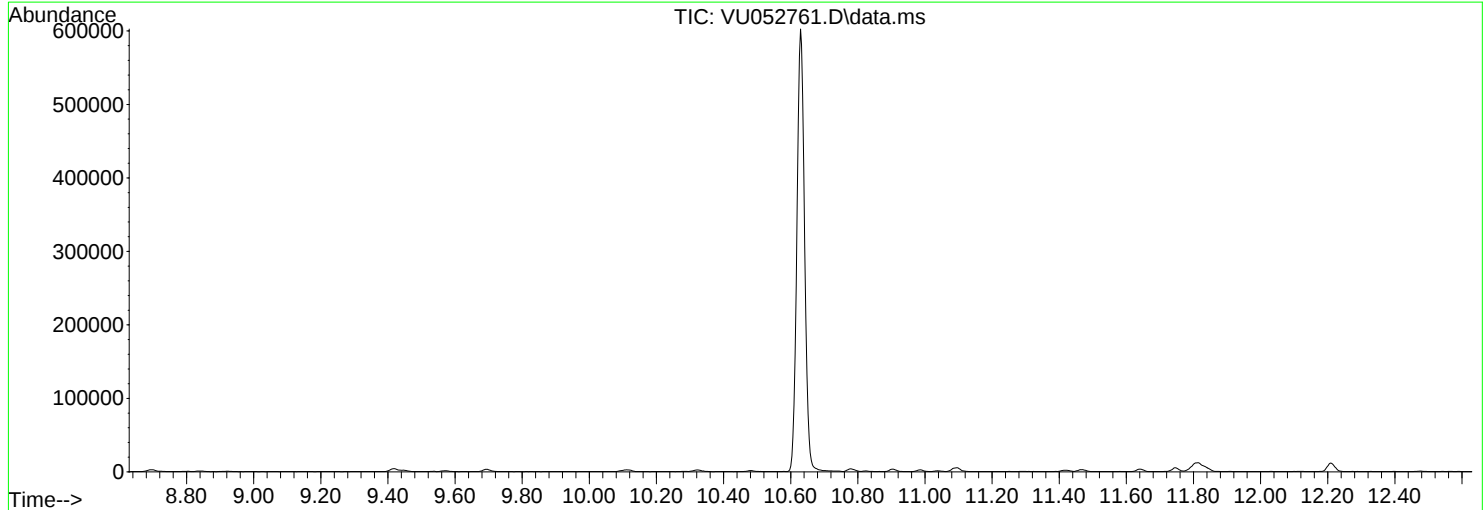

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	21256	PASS
75	95	30	80	50.5	61827	PASS
95	95	100	100	100.0	122541	PASS
96	95	5	9	6.6	8131	PASS
173	174	0.00	2	1.3	1242	PASS
174	95	50	120	79.8	97840	PASS
175	174	5	9	7.5	7351	PASS
176	174	95	101	95.9	93864	PASS
177	176	5	9	6.5	6068	PASS

m/z	Abundance
40.00	189.0
44.00	366.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
36.00	745.0
37.00	4640.0
38.00	4310.0
39.00	1886.0
40.00	223.0
44.10	737.0
45.00	897.0
46.00	143.0
47.10	1371.0
47.90	639.0
49.00	4207.0
50.00	21408.0
51.00	6751.0
51.90	271.0
55.00	261.0
56.00	1600.0
57.00	3001.0
58.10	162.0
60.00	1020.0
61.00	5612.0
62.00	5412.0
63.00	4701.0
64.00	651.0
65.10	1057.0
67.00	370.0
68.00	11782.0
69.00	11929.0
70.00	776.0
72.00	719.0
73.00	5416.0
74.00	19120.0
75.00	61160.0
76.00	5049.0
77.00	690.0
77.90	459.0
79.00	3568.0
80.00	1152.0
80.90	3653.0
81.90	993.0
85.80	138.0
87.00	4854.0
87.90	4814.0
91.00	517.0
92.00	3421.0
93.00	5315.0
94.00	13992.0
95.00	118896.0
96.00	8229.0
97.10	185.0
104.00	539.0
105.00	158.0
105.80	570.0
106.80	163.0
110.90	110.0
112.80	134.0
114.80	130.0
115.90	290.0
116.80	968.0
117.90	348.0
118.80	674.0
128.00	437.0
128.80	174.0
129.80	404.0
130.80	108.0
134.90	229.0
136.90	272.0
139.90	100.0
140.90	1217.0
141.90	155.0
142.90	1433.0
145.00	410.0
145.90	224.0
147.80	305.0
149.90	123.0
153.90	103.0
155.00	192.0
156.80	200.0
158.90	145.0
160.90	221.0
171.00	159.0
172.00	1218.0
173.00	1271.0
173.90	92376.0
175.00	7342.0
176.00	87768.0
177.00	5815.0
177.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
36.00	827.0
37.00	4760.0
38.00	4515.0
39.00	2042.0
40.00	224.0
44.00	753.0
44.90	864.0
46.00	173.0
47.00	1363.0
47.90	680.0
49.00	4517.0
50.00	21912.0
51.00	6826.0
51.90	351.0
55.00	283.0
56.00	1511.0
57.00	3278.0
58.10	124.0
60.00	1056.0
61.00	6110.0
62.00	5651.0
63.00	5015.0
64.00	617.0
65.10	1050.0
65.90	125.0
66.90	319.0
68.00	12098.0
69.00	12381.0
70.00	814.0
72.00	710.0
73.00	5687.0
74.00	20248.0
75.00	64088.0
76.00	5032.0
77.00	722.0
78.00	500.0
79.00	3747.0
80.00	1147.0
80.90	3607.0
81.90	1001.0
85.80	139.0
87.00	4879.0
87.90	4971.0
91.00	512.0
92.00	3640.0
93.00	5580.0
94.00	14463.0
95.00	126672.0
96.00	8331.0
97.00	235.0
104.00	520.0
104.90	146.0
105.90	532.0
106.80	202.0
110.90	104.0
112.00	104.0
112.80	108.0
114.80	137.0
116.00	308.0
116.90	1041.0
117.90	460.0
118.90	729.0
127.90	458.0
128.80	197.0
129.80	532.0
130.80	140.0
134.90	246.0
136.90	250.0
140.00	146.0
140.90	1267.0
141.90	195.0
142.90	1547.0
144.90	442.0
145.90	203.0
146.90	113.0
147.80	316.0
150.00	152.0
153.90	117.0
154.90	201.0
156.90	205.0
158.80	182.0
160.90	235.0
171.10	196.0
172.00	1187.0
173.00	1282.0
173.90	101144.0
175.00	7625.0
175.90	97032.0
177.00	6262.0
177.90	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192

m/z	Abundance
36.00	843.0
37.00	4467.0
38.00	4338.0
39.10	2003.0
39.90	222.0
44.00	747.0
44.90	804.0
46.00	136.0
47.10	1225.0
48.00	678.0
49.00	4383.0
50.00	20448.0
51.00	6273.0
52.00	356.0
55.00	273.0
56.00	1391.0
57.00	3219.0
60.00	1006.0
61.00	5983.0
62.00	5307.0
63.00	4795.0
64.00	546.0
65.10	914.0
65.90	130.0
67.10	287.0
68.00	11541.0
69.00	12036.0
70.00	794.0
71.90	619.0
73.00	5268.0
74.00	19536.0
75.00	60232.0
76.10	4790.0
77.00	771.0
78.10	517.0
78.90	3545.0
79.90	1069.0
80.90	3193.0
81.90	886.0
85.80	137.0
87.00	4316.0
87.90	4712.0
91.00	492.0
92.00	3532.0
93.00	5416.0
94.00	13812.0
95.00	122056.0
96.00	7834.0
96.90	255.0
103.80	487.0
104.90	148.0
105.90	500.0
106.90	197.0
112.00	110.0
114.80	114.0
116.00	330.0
116.90	1024.0
117.90	528.0
118.90	658.0
127.90	453.0
128.80	151.0
129.80	585.0
130.80	153.0
134.90	231.0
136.90	218.0
140.00	167.0
141.00	1111.0
141.90	183.0
142.90	1496.0
144.90	415.0
146.00	179.0
146.90	120.0
147.90	311.0
150.00	167.0
154.90	211.0
156.90	174.0
158.80	196.0
160.90	184.0
171.10	197.0
172.00	1054.0
173.00	1174.0
173.90	100000.0
175.00	7086.0
175.90	96792.0
177.00	6128.0
178.00	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB192