

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012125\
 Data File : VU062938.D
 Acq On : 21 Jan 2025 13:47
 Operator : MD/SY
 Sample : Q1086-16DL2 1000X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF7DL2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.473	50	57	75	rBV3	3219	6760	2.54%	0.295%
2	1.595	88	95	107	rVB	24842	27795	10.45%	1.214%
3	1.904	181	191	200	rVB	24579	30742	11.55%	1.342%
4	2.557	383	394	410	rBB	38758	61951	23.28%	2.705%
5	3.168	575	584	585	rBV	2877	3120	1.17%	0.136%
6	4.605	1022	1031	1066	rBV	41790	107451	40.38%	4.691%
7	5.049	1155	1169	1193	rBV2	59842	132598	49.83%	5.789%
8	5.303	1233	1248	1268	rBB2	32649	74559	28.02%	3.255%
9	5.711	1357	1375	1398	rBV2	98425	266075	100.00%	11.617%
10	6.238	1525	1539	1563	rBV	113966	219357	82.44%	9.577%
11	6.676	1664	1675	1697	rBV	58056	114233	42.93%	4.987%
12	7.557	1938	1949	1975	rBB	31502	55787	20.97%	2.436%
13	7.888	2040	2052	2072	rBV	104363	180401	67.80%	7.876%
14	8.171	2131	2140	2157	rBV2	17907	31385	11.80%	1.370%
15	8.621	2270	2280	2314	rBV2	100316	200183	75.24%	8.740%
16	9.405	2513	2524	2548	rBV	145190	250508	94.15%	10.937%
17	10.743	2930	2940	2960	rBB	55203	90262	33.92%	3.941%
18	11.801	3259	3269	3290	rBV	137234	236155	88.76%	10.311%
19	12.183	3377	3388	3408	rBV	116254	201092	75.58%	8.780%




Sum of corrected areas: 2290414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012125\
Data File : VU062938.D
Acq On : 21 Jan 2025 13:47
Operator : MD/SY
Sample : Q1086-16DL2 1000X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF7DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

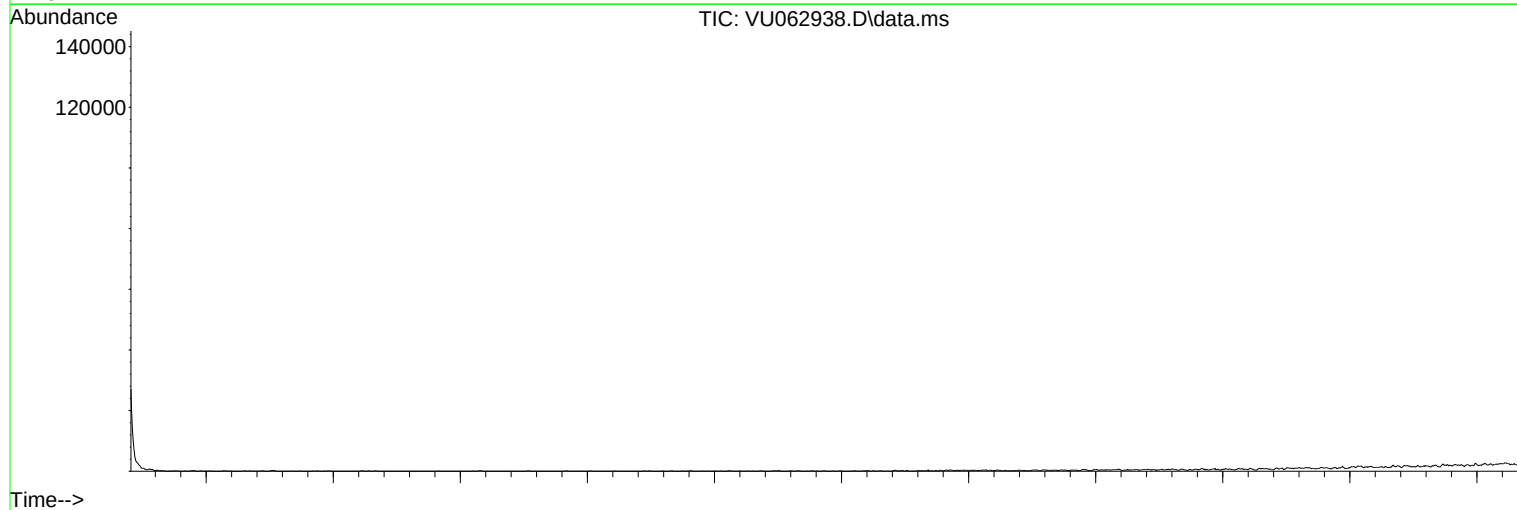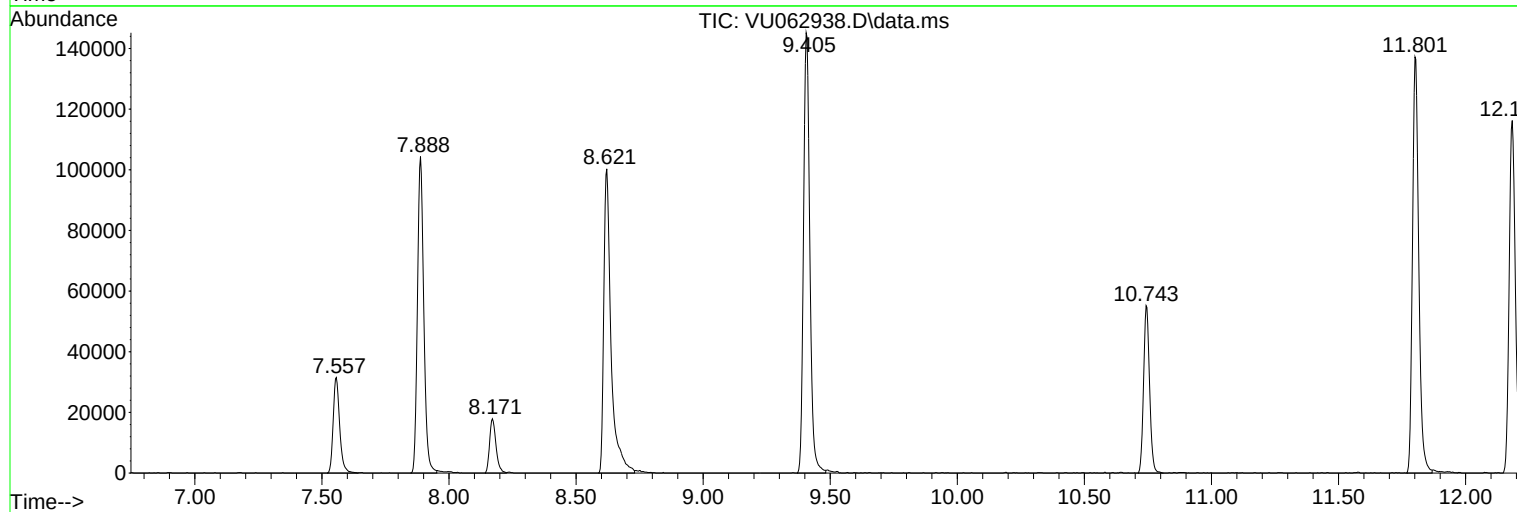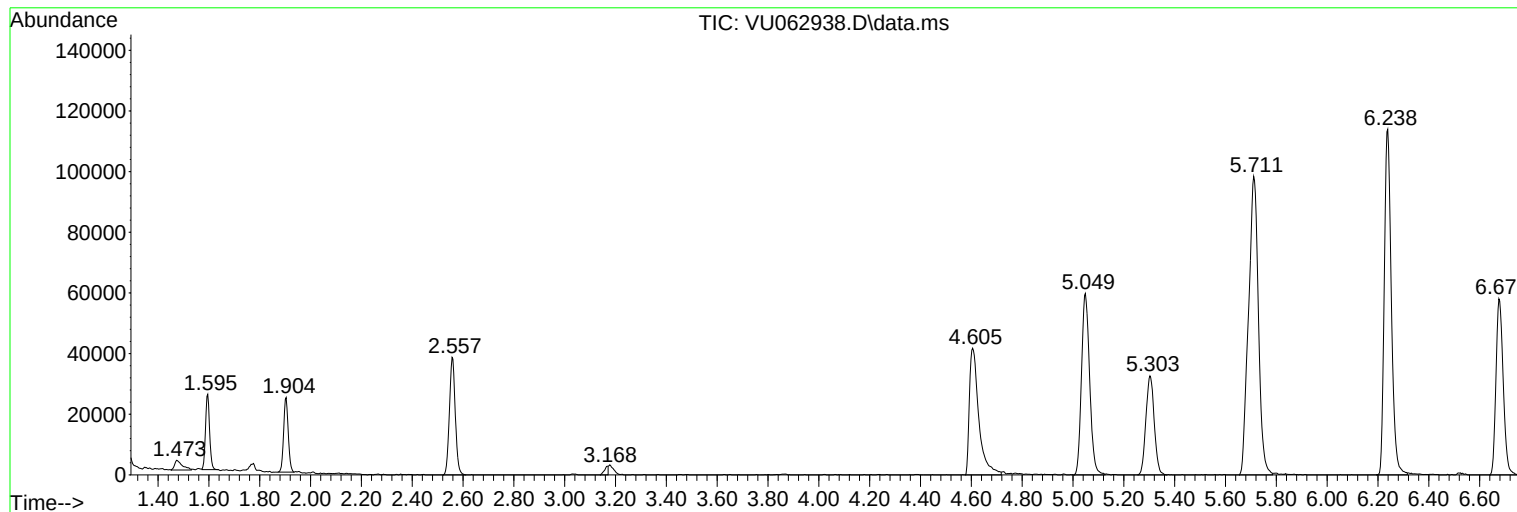

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012125\
Data File : VU062938.D
Acq On : 21 Jan 2025 13:47
Operator : MD/SY
Sample : Q1086-16DL2 1000X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF7DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012125\
Data File : VU062938.D
Acq On : 21 Jan 2025 13:47
Operator : MD/SY
Sample : Q1086-16DL2 1000X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF7DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc