
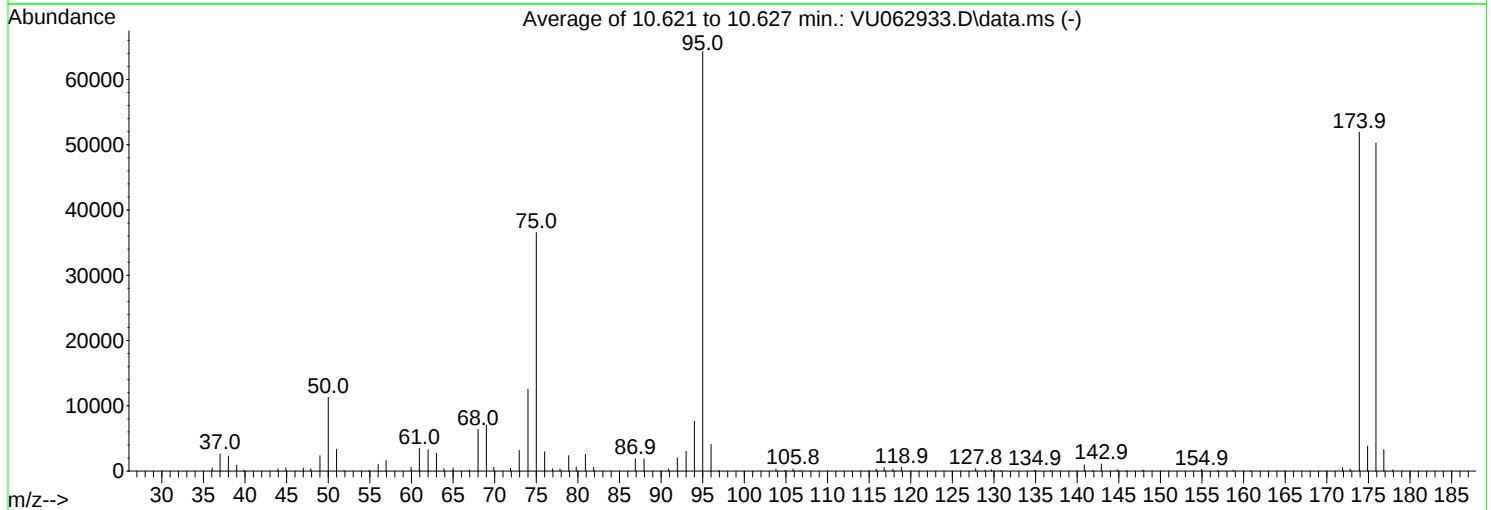


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012125\
Data File : VU062933.D
Acq On : 21 Jan 2025 09:08
Operator : MD/SY
Sample : BFB065
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB065

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 23 00:43:08 2025

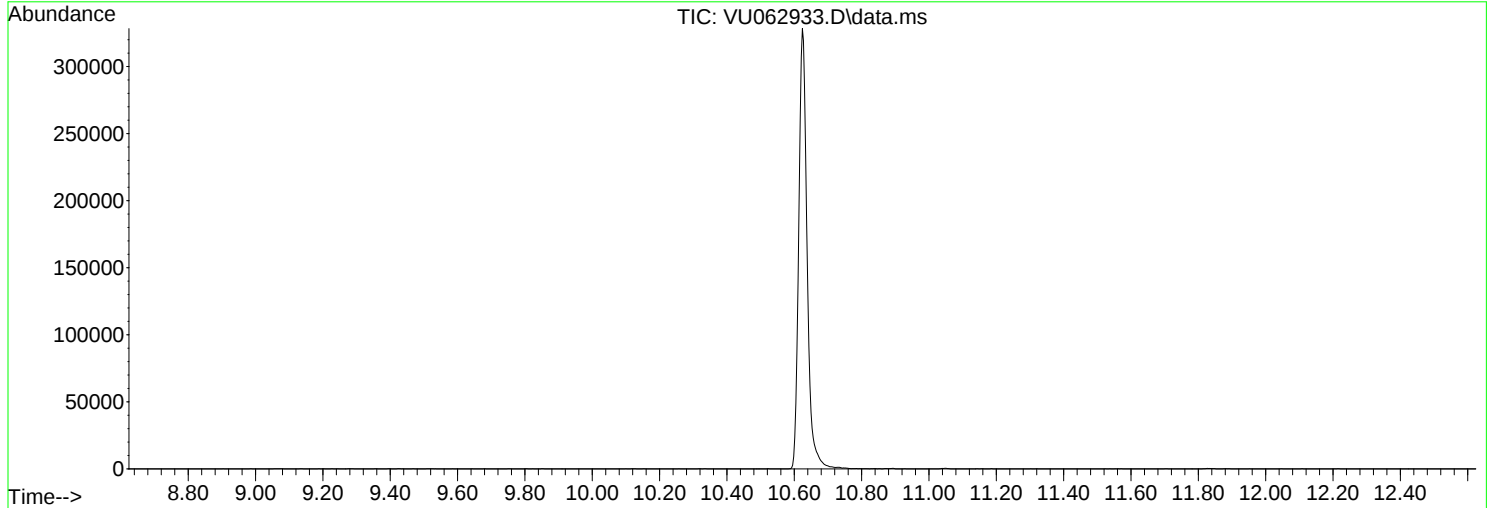

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	11321	PASS
75	95	30	80	56.9	36544	PASS
95	95	100	100	100.0	64251	PASS
96	95	5	9	6.4	4088	PASS
173	174	0.00	2	0.6	327	PASS
174	95	50	120	80.8	51933	PASS
175	174	5	9	7.4	3824	PASS
176	174	95	101	96.8	50251	PASS
177	176	5	9	6.5	3279	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB065

m/z	Abundance
36.10	415.0
37.00	2672.0
38.00	2145.0
39.00	870.0
39.80	121.0
43.90	336.0
44.90	432.0
47.00	415.0
47.90	383.0
49.00	2219.0
50.00	11032.0
51.00	3167.0
54.80	104.0
56.00	934.0
57.00	1557.0
59.90	626.0
61.00	3398.0
62.00	3191.0
63.00	2764.0
63.90	408.0
65.00	571.0
67.00	182.0
68.00	6419.0
69.00	6864.0
69.90	555.0
71.90	380.0
73.00	2952.0
74.00	12414.0
75.00	35152.0
76.00	2880.0
76.90	371.0
77.80	268.0
78.90	2204.0
79.80	630.0
80.90	2511.0
81.90	524.0
86.90	1769.0
88.00	1976.0
90.90	373.0
92.00	1940.0
93.00	2966.0
94.00	7550.0
95.00	62232.0
96.00	4039.0
96.90	131.0
103.80	241.0
104.90	130.0
105.80	278.0
106.70	110.0
115.80	339.0
116.70	512.0
117.90	394.0
118.90	524.0
127.80	376.0
129.70	201.0
134.90	132.0
136.90	105.0
140.90	903.0
141.80	135.0
142.90	1110.0
144.80	179.0
145.90	111.0
147.90	164.0
154.90	270.0
158.80	136.0
160.90	160.0
171.90	527.0
172.80	488.0
173.90	49496.0
174.90	3656.0
175.90	48144.0
176.80	3211.0
177.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	473.0
37.00	2707.0
38.00	2354.0
39.00	964.0
39.80	132.0
44.00	378.0
44.90	511.0
47.00	500.0
47.90	385.0
49.00	2416.0
50.00	11771.0
51.00	3403.0
51.90	119.0
54.90	127.0
56.00	1097.0
56.90	1662.0
59.90	611.0
61.00	3636.0
62.00	3382.0
63.00	2802.0
63.90	388.0
65.00	512.0
66.90	189.0
68.00	6565.0
69.00	7305.0
69.90	594.0
71.90	427.0
73.00	3265.0
74.00	12971.0
75.00	37648.0
76.00	3007.0
76.90	337.0
77.90	365.0
78.90	2433.0
79.80	665.0
80.90	2648.0
81.90	582.0
86.90	1956.0
88.00	1906.0
90.90	352.0
92.00	2082.0
93.00	3129.0
94.00	7799.0
95.00	66224.0
96.00	4228.0
96.90	107.0
103.80	339.0
104.80	101.0
105.90	345.0
106.70	136.0
115.80	302.0
116.80	575.0
117.80	339.0
118.90	600.0
127.80	393.0
128.90	123.0
129.70	201.0
130.80	115.0
134.90	162.0
136.80	131.0
140.90	1000.0
141.80	130.0
142.90	1113.0
144.80	201.0
145.90	117.0
147.90	210.0
155.00	273.0
156.90	127.0
158.70	133.0
160.80	136.0
171.90	569.0
172.80	492.0
173.90	53504.0
174.90	3958.0
175.90	51744.0
176.80	3381.0
177.90	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	521.0
37.00	2569.0
38.00	2317.0
39.00	920.0
39.90	123.0
44.00	346.0
44.90	508.0
47.00	453.0
47.90	348.0
49.00	2448.0
50.00	11161.0
51.00	3353.0
51.90	127.0
55.00	162.0
56.00	1116.0
56.90	1637.0
60.00	603.0
60.90	3448.0
62.00	3240.0
63.00	2654.0
63.90	350.0
65.00	426.0
66.90	140.0
68.00	6253.0
69.00	7001.0
69.90	574.0
71.90	445.0
72.90	3239.0
74.00	12362.0
75.00	36832.0
76.00	2952.0
77.00	323.0
77.90	354.0
78.90	2477.0
79.80	681.0
80.90	2596.0
81.90	613.0
86.90	1940.0
87.90	1732.0
90.90	299.0
91.90	2107.0
93.00	3026.0
94.00	7519.0
95.00	64296.0
96.00	3998.0
103.80	395.0
105.90	412.0
106.70	102.0
115.00	114.0
115.90	299.0
116.90	674.0
117.80	259.0
118.90	639.0
127.80	371.0
128.90	123.0
129.70	201.0
130.80	120.0
134.90	190.0
136.70	178.0
140.80	994.0
141.90	110.0
142.90	1053.0
144.80	233.0
147.90	195.0
155.00	225.0
156.90	169.0
158.70	104.0
171.90	513.0
173.90	52800.0
174.90	3858.0
175.90	50864.0
176.90	3246.0
177.90	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065