


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU012220\
 Data File : VU036523.D
 Acq On : 22 Jan 2020 13:46
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jan 23 08:59:25 2020

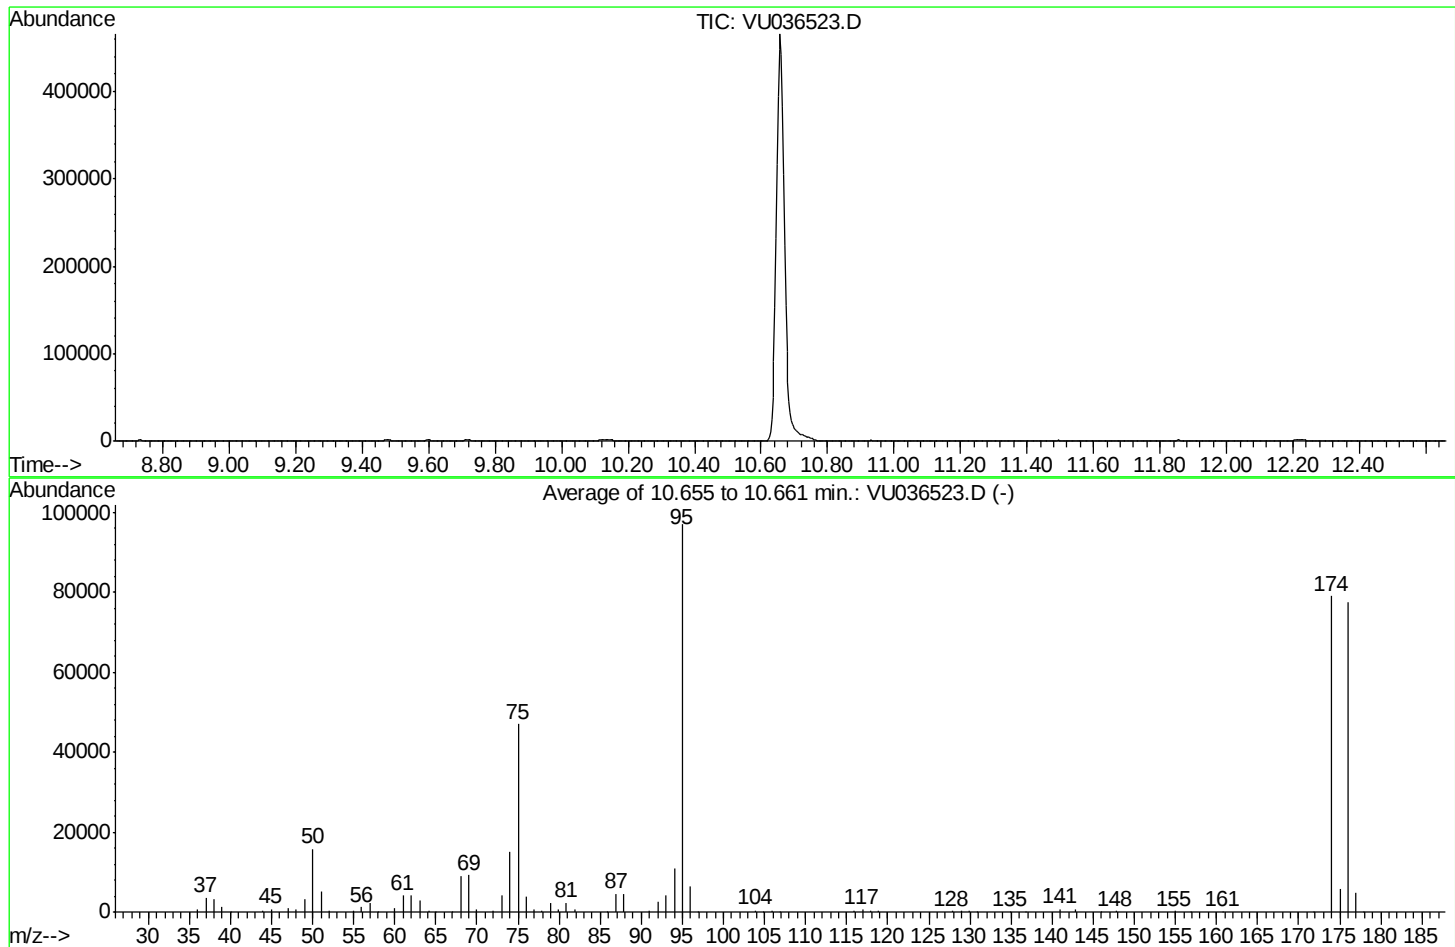

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	15811	PASS
75	95	30	60	48.4	46960	PASS
95	95	100	100	100.0	97042	PASS
96	95	5	9	6.6	6419	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.5	79082	PASS
175	174	5	9	7.3	5792	PASS
176	174	95	101	98.2	77626	PASS
177	176	5	9	6.3	4864	PASS