

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012221\
 Data File : VU042180.D
 Acq On : 22 Jan 2021 19:22
 Operator : SY/MD
 Sample : M1222-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F1E33

Quant Time: Jan 23 06:25:58 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 23 06:18:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	96132	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	90290	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	49068	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	24092	3.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.60%
7) Chloroethane-d5	1.916	69	22434	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.571	63	45764	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	4.652	46	124862	55.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.36%
24) Chloroform-d	5.073	84	63074	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.710	65	39756	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
32) Benzene-d6	5.735	84	115142	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.700	67	38111	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.906	98	105962	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloroprop...	8.189	79	18117	4.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.00%
46) 2-Hexanone-d5	8.645	63	90562	53.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.92%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	34190	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.80%
64) 1,2-Dichlorobenzene-d4	12.201	152	44575	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%
Target Compounds					Qvalue	
42) Toluene	7.976	91	1939	0.07	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012221\
Data File : VU042180.D
Acq On : 22 Jan 2021 19:22
Operator : SY/MD
Sample : M1222-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F1E33

Quant Time: Jan 23 06:25:58 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 23 06:18:59 2021
Response via : Initial Calibration

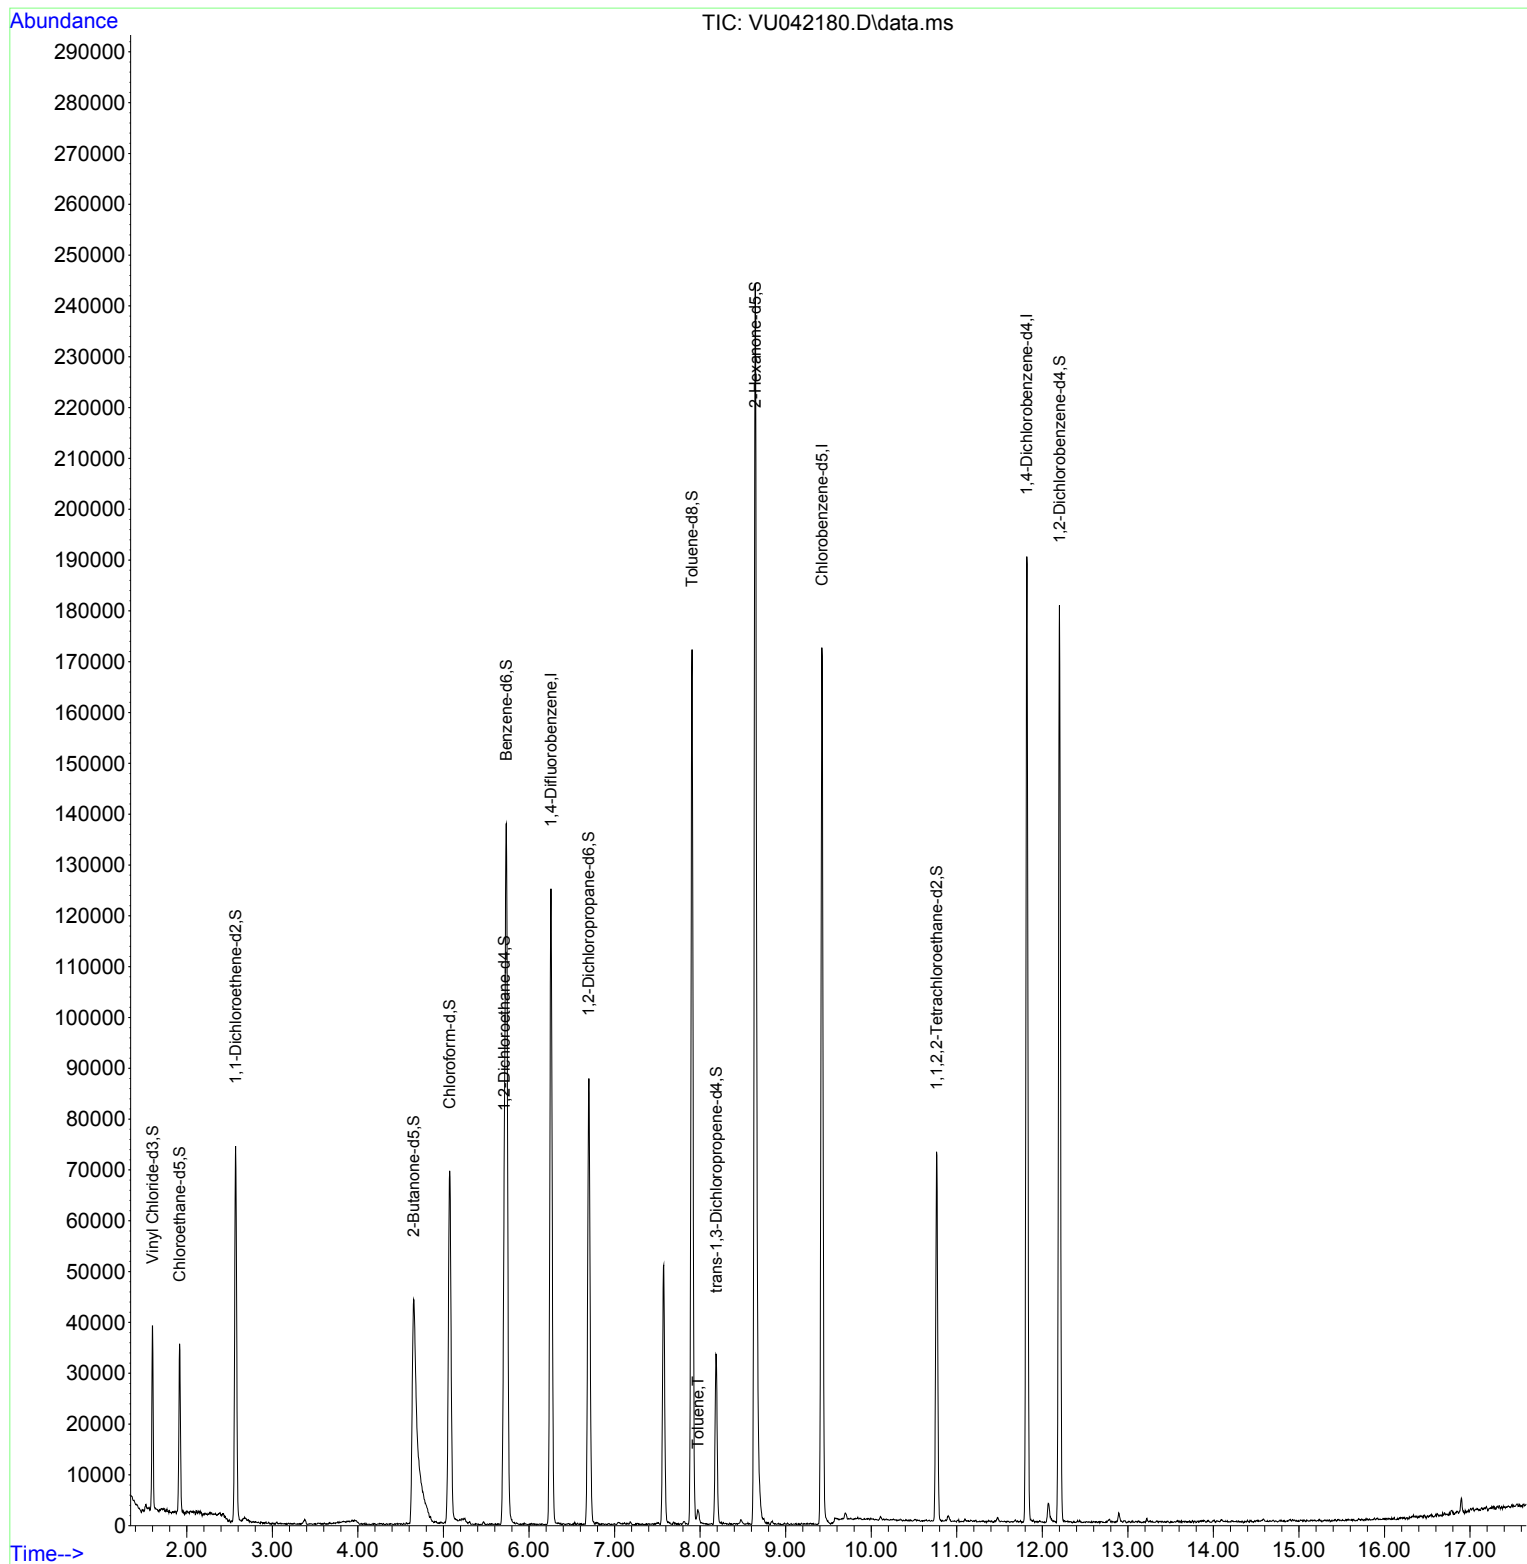


Abundance Scan 2064 (7.977 min): VU042162.D\data.ms (-2

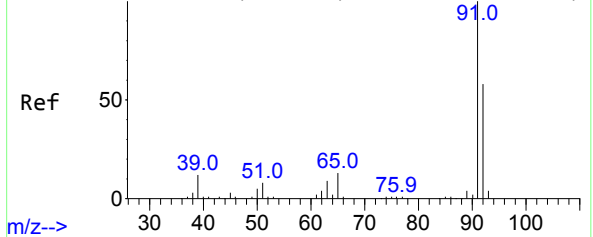

#42
Toluene
Concen: 0.07 ug/L
RT: 7.976 min Scan# 2064
Delta R.T. -0.000 min
Lab File: VU042180.D
Acq: 22 Jan 2021 19:22

Instrument :
MSVOA_U
ClientSampleId :
F1E33

Abundance Scan 2064 (7.976 min): VU042180.D\data.ms

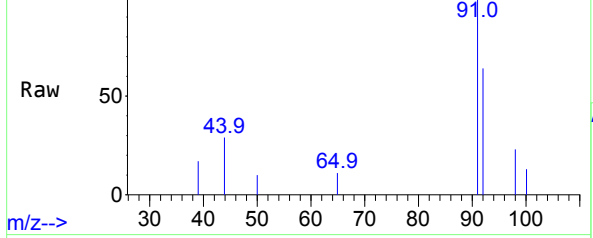

Tgt Ion: 91 Resp: 1939
Ion Ratio Lower Upper
91 100
92 64.3 41.2 76.6

Abundance Scan 2064 (7.976 min): VU042180.D\data.ms (-1

