
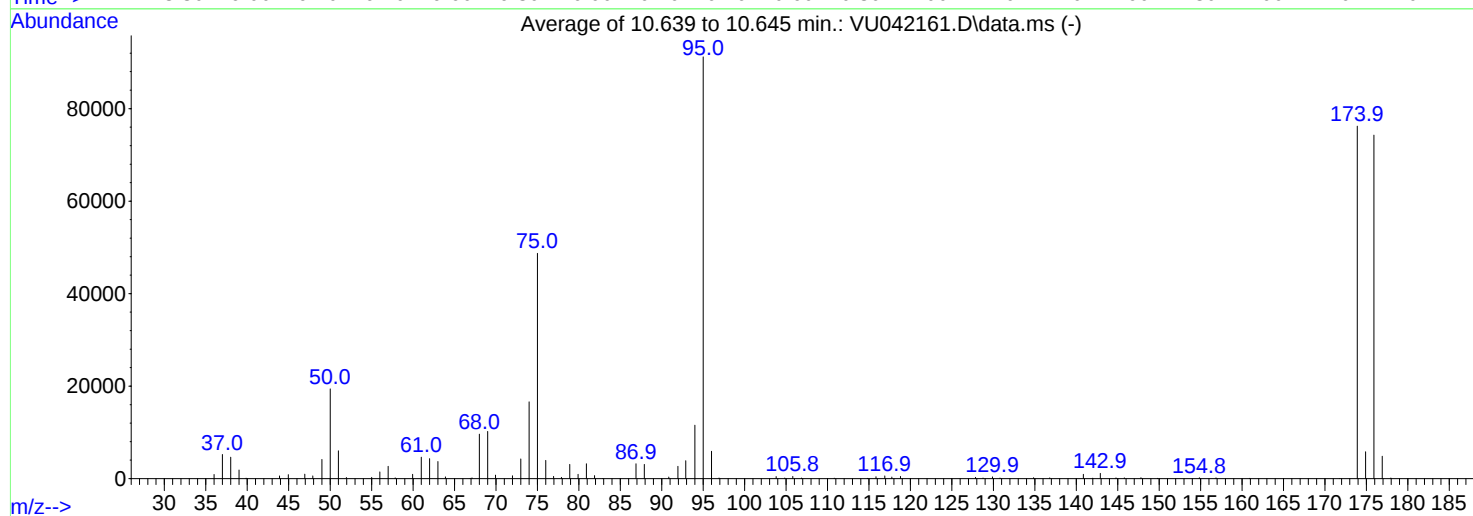


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012221\
 Data File : VU042161.D
 Acq On : 22 Jan 2021 09:31
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 23 06:18:59 2021

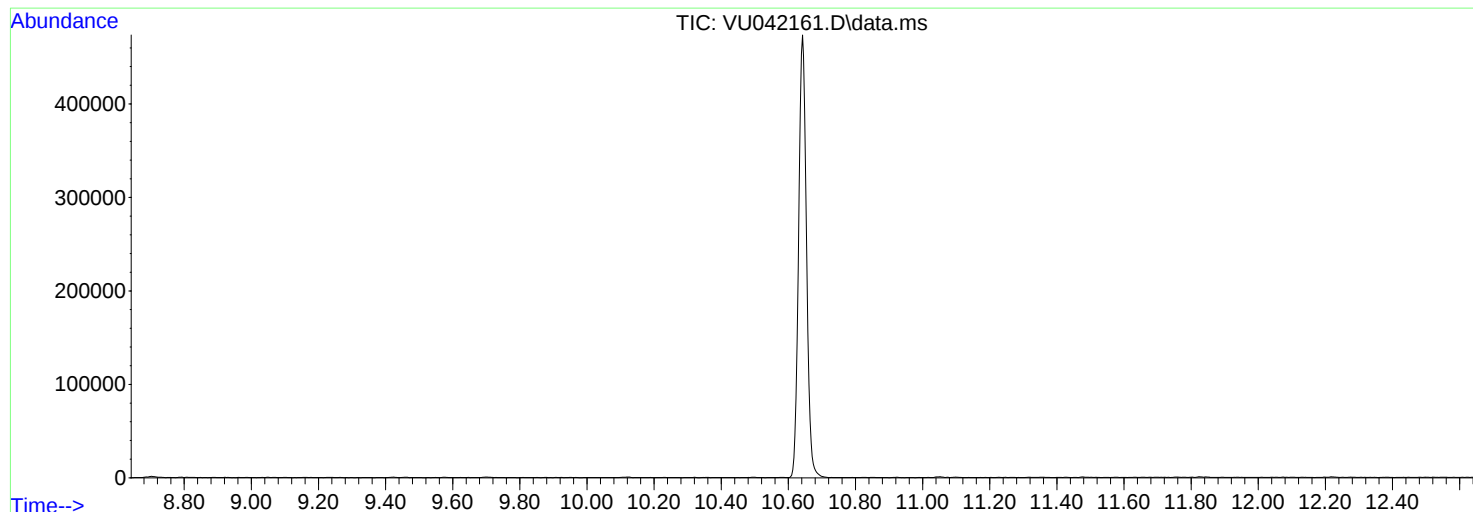

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	19397	PASS
75	95	30	80	53.4	48717	PASS
95	95	100	100	100.0	91205	PASS
96	95	5	9	6.5	5901	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	76224	PASS
175	174	5	9	7.6	5815	PASS
176	174	95	101	97.4	74272	PASS
177	176	5	9	6.5	4858	PASS

m/z	Abundance
36.00	901.0
37.00	5309.0
38.00	4725.0
39.00	1928.0
39.80	118.0
43.90	903.0
45.00	826.0
47.00	1001.0
47.90	635.0
49.00	4136.0
50.00	19608.0
51.00	6001.0
51.90	252.0
55.00	315.0
56.00	1466.0
57.00	2649.0
57.80	143.0
60.00	949.0
61.00	4677.0
62.00	4456.0
63.00	3509.0
63.90	396.0
66.90	234.0
68.00	9467.0
69.00	10331.0
70.00	811.0
72.00	628.0
73.00	4169.0
74.00	16568.0
75.00	48288.0
76.00	4050.0
77.00	529.0
77.90	308.0
78.90	3035.0
79.90	968.0
80.90	3229.0
81.90	695.0
86.90	3133.0
87.90	3040.0
90.90	387.0
91.90	2699.0
92.90	3830.0
94.00	11577.0
95.00	90816.0
96.00	5954.0
96.90	122.0
103.80	440.0
104.80	151.0
105.80	441.0
106.90	111.0
110.80	100.0
114.80	111.0
115.90	448.0
116.90	598.0
117.70	307.0
118.80	497.0
127.90	286.0
128.70	140.0
129.90	436.0
130.80	116.0
134.80	194.0
136.80	162.0
140.80	945.0
142.00	131.0
142.90	1119.0
144.80	128.0
145.80	172.0
147.80	182.0
154.80	197.0
156.90	165.0
171.80	151.0
173.90	73808.0
174.90	5671.0
175.90	71640.0
176.90	4739.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	916.0
37.00	5362.0
38.00	4799.0
39.00	1955.0
39.90	110.0
43.90	976.0
45.00	887.0
47.00	1013.0
47.90	602.0
49.00	4287.0
50.00	19952.0
51.00	6188.0
52.00	252.0
55.00	291.0
56.00	1481.0
57.00	2718.0
57.80	189.0
59.90	975.0
61.00	4739.0
62.00	4430.0
63.00	3815.0
63.90	381.0
67.10	227.0
68.00	9926.0
69.00	10592.0
69.90	768.0
72.00	645.0
73.00	4353.0
74.00	17128.0
75.00	50208.0
76.00	4061.0
77.00	496.0
77.90	299.0
78.90	3181.0
79.90	987.0
80.90	3334.0
81.90	656.0
82.90	102.0
86.90	3271.0
87.90	3171.0
90.90	378.0
92.00	2710.0
92.90	3979.0
94.00	11945.0
95.00	94008.0
96.00	6099.0
96.90	134.0
103.80	471.0
104.90	155.0
105.80	539.0
106.80	153.0
110.80	131.0
114.80	113.0
115.80	434.0
116.90	618.0
117.80	346.0
118.80	491.0
127.90	300.0
128.80	129.0
129.90	422.0
130.80	142.0
134.80	220.0
136.80	173.0
140.90	966.0
142.00	130.0
142.90	1207.0
144.80	183.0
145.80	198.0
147.80	207.0
149.80	117.0
154.90	220.0
156.90	182.0
160.90	114.0
173.90	78656.0
174.90	5991.0
175.90	76584.0
176.90	5040.0
178.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	846.0
37.00	4968.0
38.00	4391.0
39.00	1750.0
39.90	108.0
44.00	927.0
44.90	888.0
46.90	933.0
47.90	525.0
49.00	4074.0
50.00	18632.0
51.00	5850.0
52.00	224.0
55.00	242.0
56.00	1416.0
57.00	2611.0
57.90	182.0
59.90	871.0
61.00	4486.0
62.00	4110.0
63.00	3764.0
63.90	326.0
67.10	260.0
68.00	9502.0
69.00	9750.0
70.00	678.0
72.00	571.0
73.00	4222.0
74.00	16183.0
75.00	47656.0
76.00	3711.0
76.90	413.0
77.90	276.0
78.90	3020.0
79.90	911.0
80.90	3098.0
81.90	621.0
86.90	3230.0
87.90	3015.0
90.80	328.0
92.00	2565.0
92.90	3777.0
94.00	11133.0
95.00	88792.0
96.00	5650.0
96.90	139.0
103.80	476.0
104.90	128.0
105.80	525.0
106.80	158.0
110.80	108.0
115.80	371.0
116.90	598.0
117.80	380.0
118.80	449.0
127.80	300.0
128.80	123.0
129.90	332.0
130.80	150.0
134.90	221.0
136.80	157.0
140.90	946.0
142.00	106.0
142.90	1119.0
144.80	192.0
145.80	182.0
147.80	196.0
149.80	106.0
154.90	226.0
156.80	196.0
160.90	146.0
173.90	76208.0
174.90	5784.0
175.90	74592.0
176.90	4795.0
177.90	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
43.90	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40