
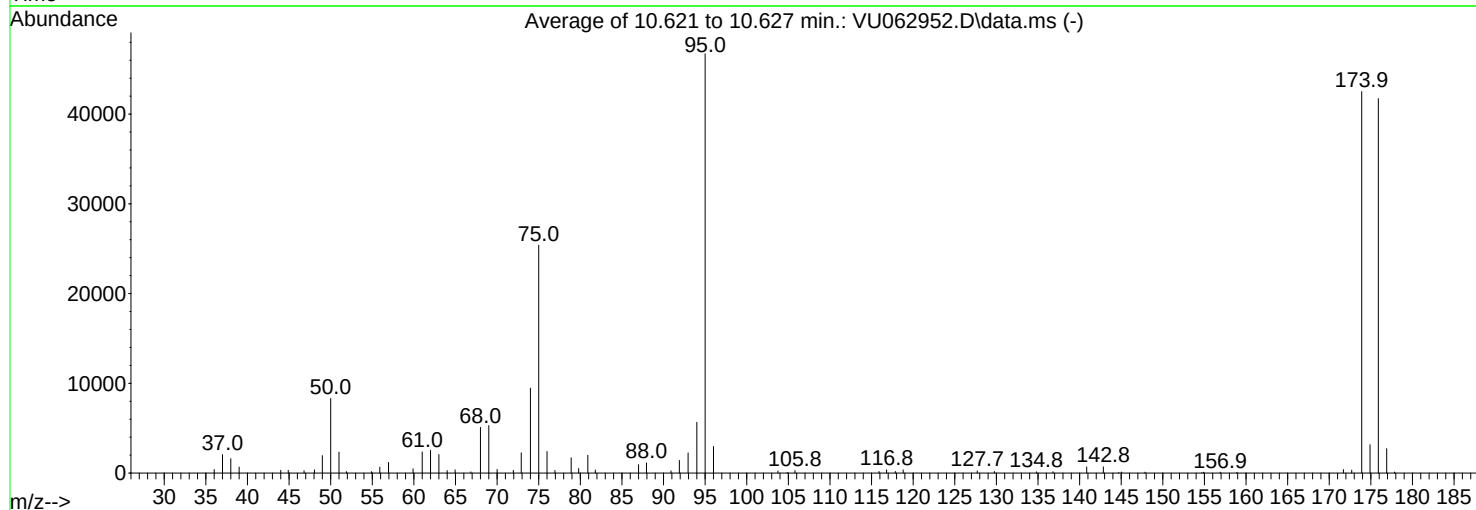


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012225\
Data File : VU062952.D
Acq On : 22 Jan 2025 08:36
Operator : MD/SY
Sample : BFB066
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB066

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 23 00:43:08 2025

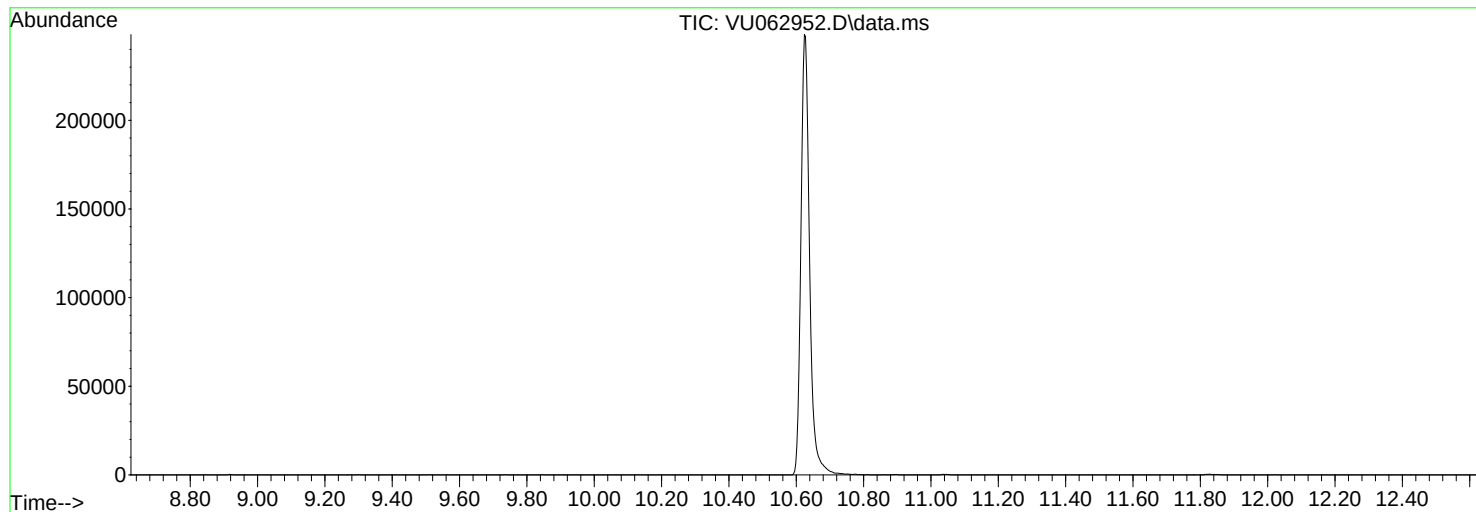

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	8312	PASS
75	95	30	80	54.4	25400	PASS
95	95	100	100	100.0	46723	PASS
96	95	5	9	6.3	2958	PASS
173	174	0.00	2	0.8	334	PASS
174	95	50	120	91.0	42507	PASS
175	174	5	9	7.4	3163	PASS
176	174	95	101	98.2	41725	PASS
177	176	5	9	6.5	2717	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB066

m/z	Abundance
36.00	371.0
37.00	2032.0
38.00	1563.0
39.00	619.0
44.00	307.0
44.90	301.0
46.80	237.0
48.00	338.0
49.00	1925.0
50.00	7952.0
51.00	2242.0
51.90	184.0
54.80	157.0
55.90	578.0
56.90	1123.0
59.90	505.0
61.00	2415.0
62.00	2521.0
63.00	1858.0
64.10	274.0
64.90	281.0
66.80	150.0
68.00	4884.0
69.00	4890.0
70.00	376.0
72.00	269.0
72.90	2049.0
74.00	8750.0
75.00	24352.0
76.00	2319.0
77.00	214.0
78.90	1600.0
79.80	440.0
80.90	1871.0
81.90	344.0
87.00	850.0
87.90	1015.0
90.90	214.0
91.90	1388.0
93.00	2202.0
94.00	5637.0
95.00	44800.0
96.00	2851.0
103.80	249.0
105.80	237.0
115.90	178.0
116.80	343.0
117.80	193.0
118.80	333.0
127.70	225.0
129.70	167.0
134.80	120.0
136.90	159.0
140.80	690.0
142.90	678.0
145.10	165.0
147.90	100.0
154.70	135.0
158.90	114.0
171.70	385.0
172.70	311.0
173.90	39752.0
174.90	3023.0
175.90	38560.0
176.90	2506.0
177.80	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
36.00	430.0
37.00	2120.0
38.00	1674.0
39.00	698.0
44.00	334.0
44.90	297.0
46.80	293.0
48.10	407.0
49.00	2027.0
50.00	8641.0
51.00	2431.0
51.90	182.0
54.90	173.0
55.90	687.0
57.00	1229.0
59.90	484.0
61.00	2405.0
62.00	2617.0
63.00	2150.0
64.00	280.0
65.00	376.0
66.90	142.0
68.00	5228.0
69.00	5471.0
70.00	437.0
72.00	320.0
72.90	2316.0
74.00	9787.0
75.00	26048.0
76.00	2491.0
76.90	305.0
78.90	1736.0
79.80	538.0
80.90	2033.0
81.80	361.0
87.00	943.0
88.00	1146.0
90.90	252.0
91.90	1462.0
92.90	2333.0
94.00	5747.0
95.00	48096.0
96.00	3046.0
103.80	231.0
104.80	103.0
105.80	293.0
115.90	189.0
116.80	372.0
117.90	184.0
118.80	369.0
127.70	257.0
129.80	189.0
134.80	158.0
136.80	173.0
140.80	717.0
142.80	707.0
145.00	194.0
147.90	106.0
154.90	148.0
156.90	124.0
158.90	113.0
171.70	388.0
172.70	340.0
173.90	43600.0
174.90	3192.0
175.90	43048.0
176.90	2804.0
177.90	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
36.00	402.0
37.00	2013.0
38.00	1589.0
39.00	697.0
44.00	300.0
44.90	317.0
46.80	275.0
48.10	339.0
49.00	1896.0
50.00	8344.0
51.00	2369.0
51.90	132.0
55.00	170.0
55.90	720.0
57.00	1198.0
59.90	476.0
61.00	2253.0
62.00	2470.0
63.00	2186.0
63.90	291.0
65.00	431.0
66.90	125.0
68.00	5162.0
69.00	5511.0
70.00	413.0
71.90	341.0
72.90	2409.0
74.00	9855.0
75.00	25800.0
76.00	2417.0
76.90	356.0
78.90	1769.0
79.80	546.0
80.90	2030.0
81.70	354.0
87.00	1043.0
88.00	1223.0
90.90	280.0
91.90	1396.0
92.90	2200.0
94.00	5609.0
95.00	47272.0
96.00	2977.0
103.70	230.0
104.90	108.0
105.80	321.0
115.90	185.0
116.80	385.0
117.80	188.0
118.80	386.0
127.70	261.0
129.80	202.0
134.80	155.0
136.70	157.0
140.90	635.0
142.90	704.0
144.70	177.0
147.80	122.0
154.90	150.0
156.90	175.0
171.70	405.0
172.70	351.0
173.90	44168.0
174.90	3275.0
175.90	43568.0
176.90	2841.0
177.90	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066