

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036533.D
 Acq On : 23 Jan 2020 11:00
 Operator : JC/MD
 Sample : VU0123WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0123WBL01

Quant Time: Jan 24 01:07:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jan 23 08:59:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	6.16	96	34241	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.66	95	12224	0.95	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.00%	
68) 1,2-Dichlorobenzene-d4	12.22	152	11927	0.90	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036533.D
Acq On : 23 Jan 2020 11:00
Operator : JC/MD
Sample : VU0123WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0123WBL01

Quant Time: Jan 24 01:07:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jan 23 08:59:25 2020
Response via : Initial Calibration

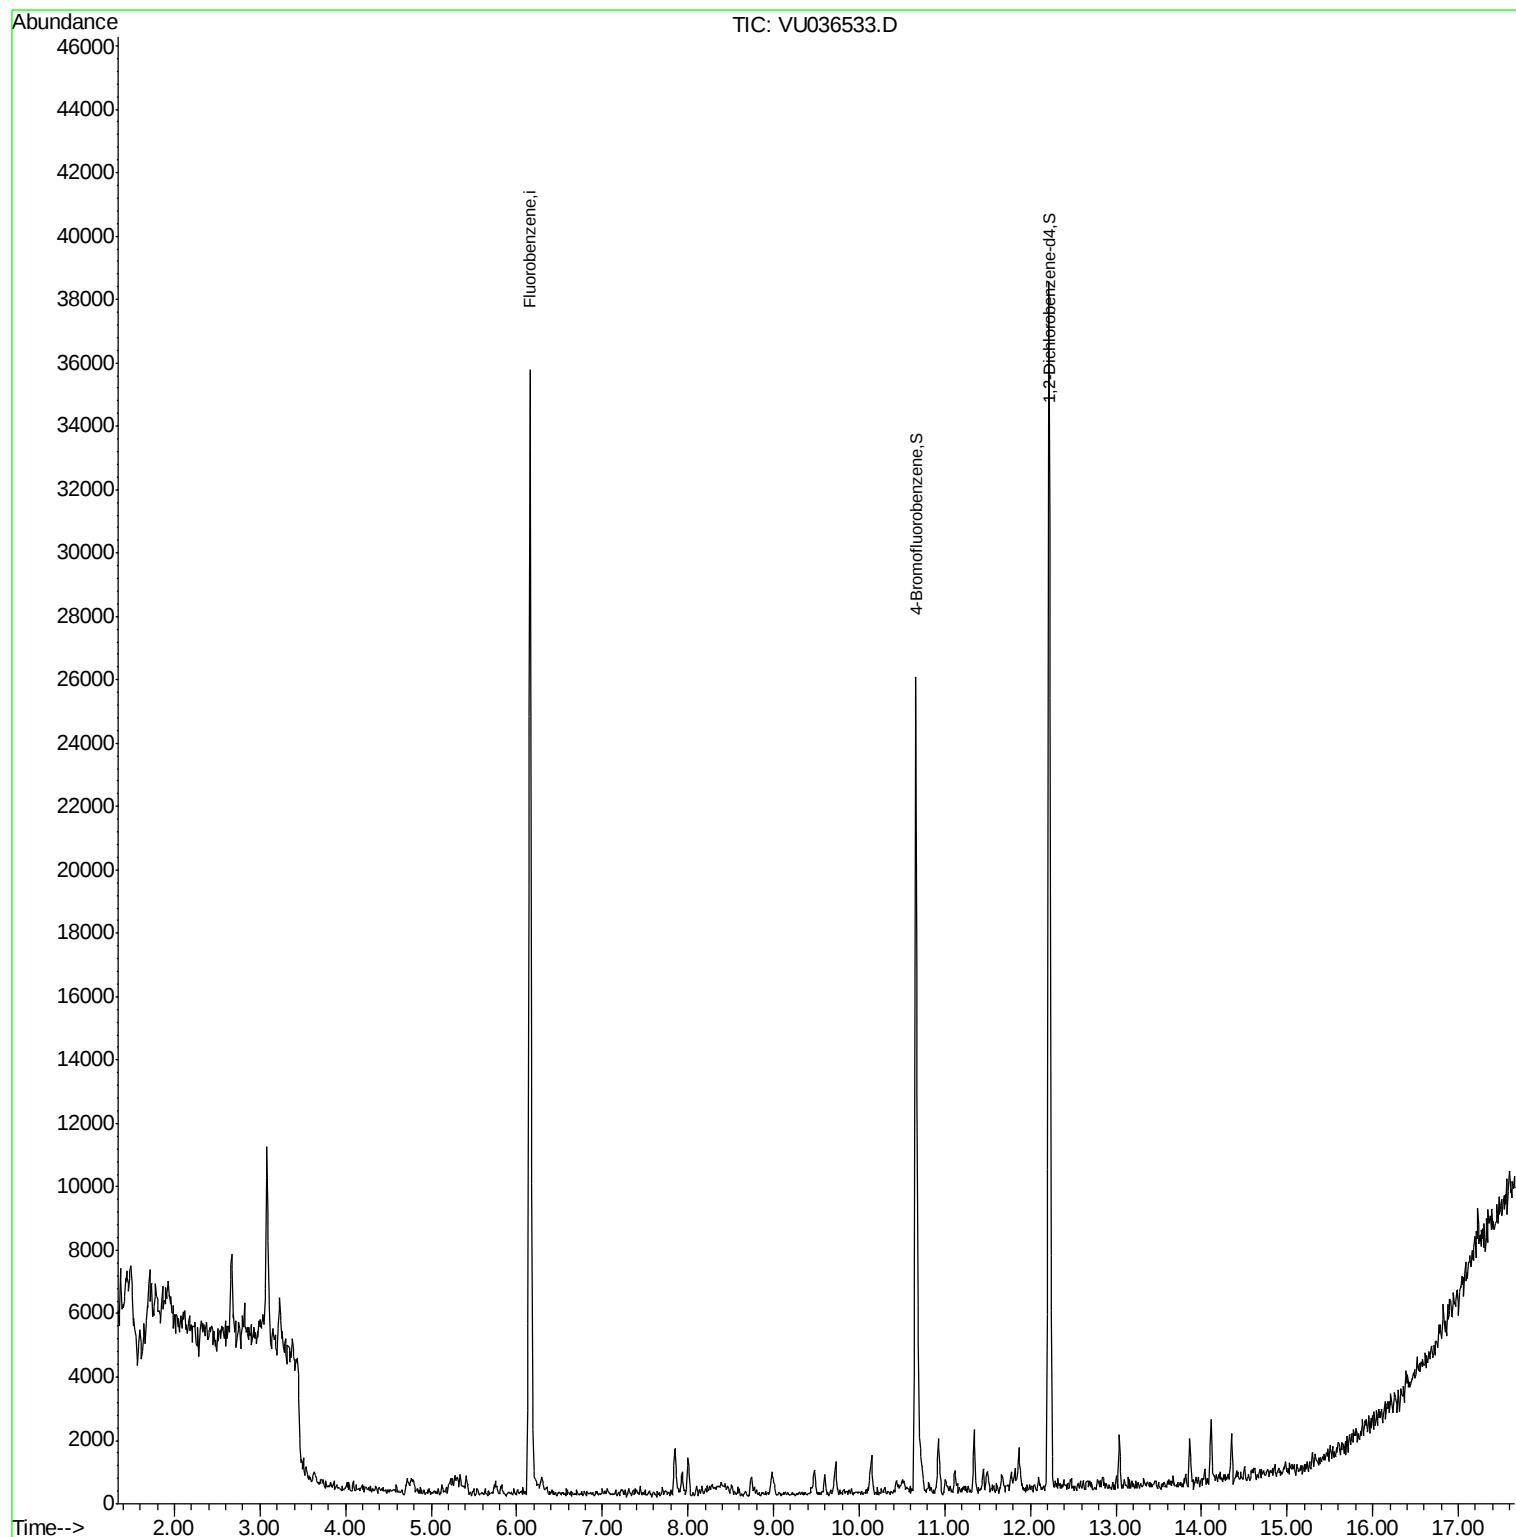

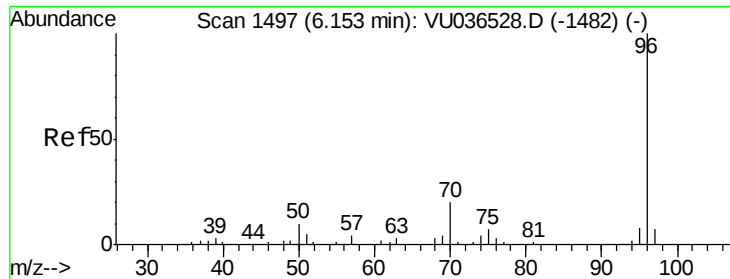

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.16 min Scan# 1498

Delta R.T. 0.00 min

Lab File: VU036533.D

Acq: 23 Jan 2020 11:00

Instrument :

MSVOA_U


ClientSampleId :

VU0123WBL01

Tot Ion: 96 Resp: 34241

Ion Ratio Lower Upper

96	100		
70	20.8	15.6	23.4
95	9.0	7.0	10.6
97	6.2	0.0	0.0#



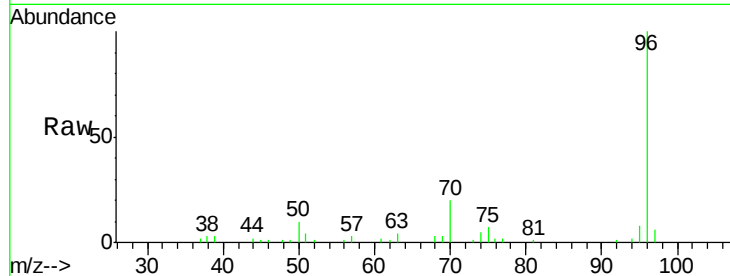


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

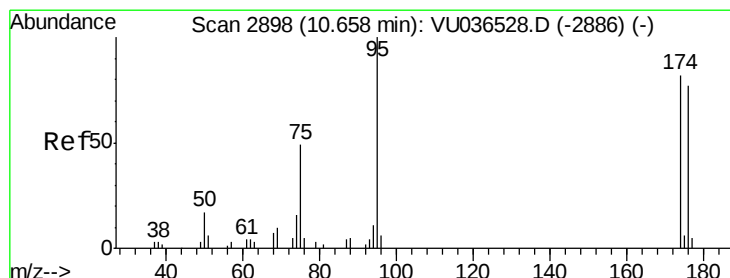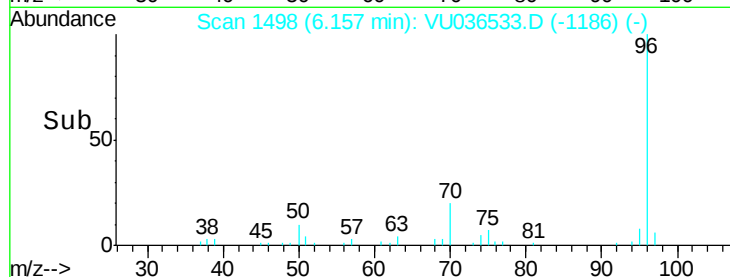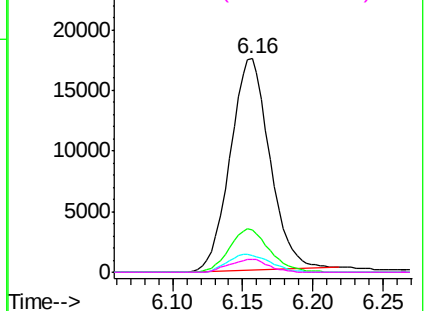

#57

4-Bromofluorobenzene

Concen: 0.946 ug/l

RT: 10.66 min Scan# 2900

Delta R.T. 0.01 min


Lab File: VU036533.D

Acq: 23 Jan 2020 11:00

Tgt Ion: 95 Resp: 12224

Ion Ratio Lower Upper



95	100		
174	72.1	64.7	97.1
176	72.1	60.6	91.0

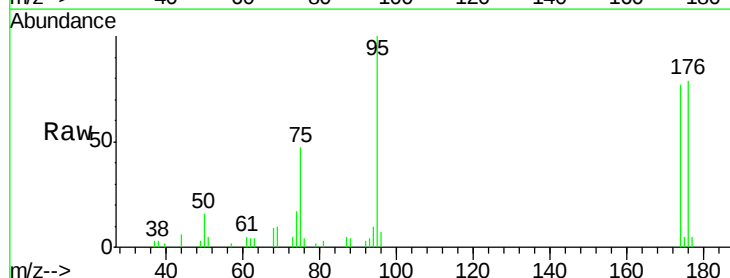


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

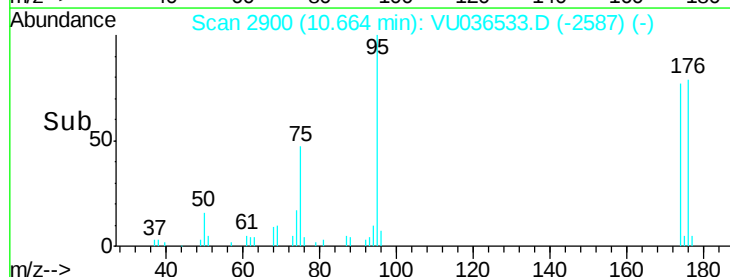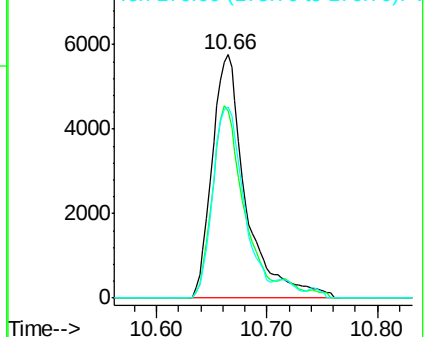


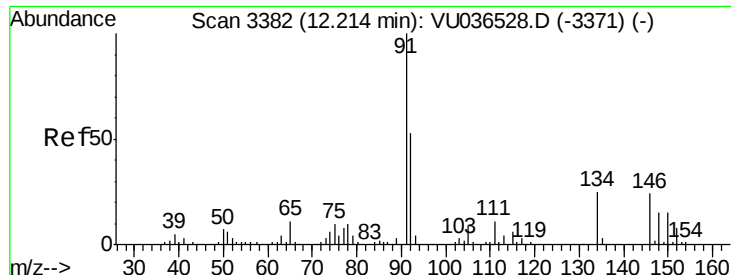

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.901 ug/l
 RT: 12.22 min Scan# 3383
 Delta R.T. 0.00 min
 Lab File: VU036533.D
 Acq: 23 Jan 2020 11:00

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0123WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	62.5	0.0	241.8
150	154.4	0.0	652.4

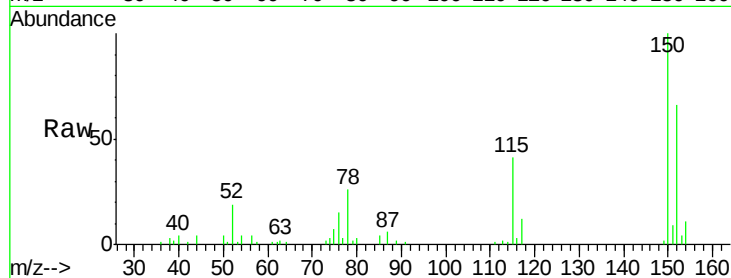

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

