

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036533.D
 Acq On : 23 Jan 2020 11:00
 Operator : JC/MD
 Sample : VU0123WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0123WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.083	536	542	558	rVB3	6379	11236	16.08%	4.889%
2	5.411	1261	1266	1277	rVB3	609	989	1.42%	0.430%
3	6.153	1484	1497	1514	rBV	35501	69477	99.45%	30.229%
4	7.848	2014	2024	2033	rBV4	1452	2706	3.87%	1.177%
5	8.002	2062	2072	2081	rVB2	1166	2021	2.89%	0.879%
6	8.742	2294	2302	2308	rBV3	599	1125	1.61%	0.489%
7	9.481	2529	2532	2538	rVB3	732	776	1.11%	0.338%
8	9.726	2598	2608	2614	rBV3	981	1538	2.20%	0.669%
9	10.144	2727	2738	2748	rVB5	1237	2236	3.20%	0.973%
10	10.661	2889	2899	2922	rBV	25627	49617	71.02%	21.588%
11	10.925	2975	2981	2990	rBV4	1432	1944	2.78%	0.846%
12	11.118	3033	3041	3048	rBV4	682	1160	1.66%	0.505%
13	11.343	3103	3111	3121	rBV3	1988	2807	4.02%	1.221%
14	11.494	3150	3158	3166	rBV2	564	965	1.38%	0.420%
15	11.864	3269	3273	3283	rVB4	1215	1579	2.26%	0.687%
16	12.217	3366	3383	3399	rBV2	38181	69864	100.00%	30.397%
17	13.041	3631	3639	3647	rVB4	1719	2419	3.46%	1.052%
18	13.860	3888	3894	3903	rBV4	1498	2130	3.05%	0.927%
19	14.111	3964	3972	3980	rBV2	2048	3038	4.35%	1.322%
20	14.352	4040	4047	4053	rVB4	1585	2209	3.16%	0.961%


Sum of corrected areas: 229836

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036533.D
Acq On : 23 Jan 2020 11:00
Operator : JC/MD
Sample : VU0123WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0123WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

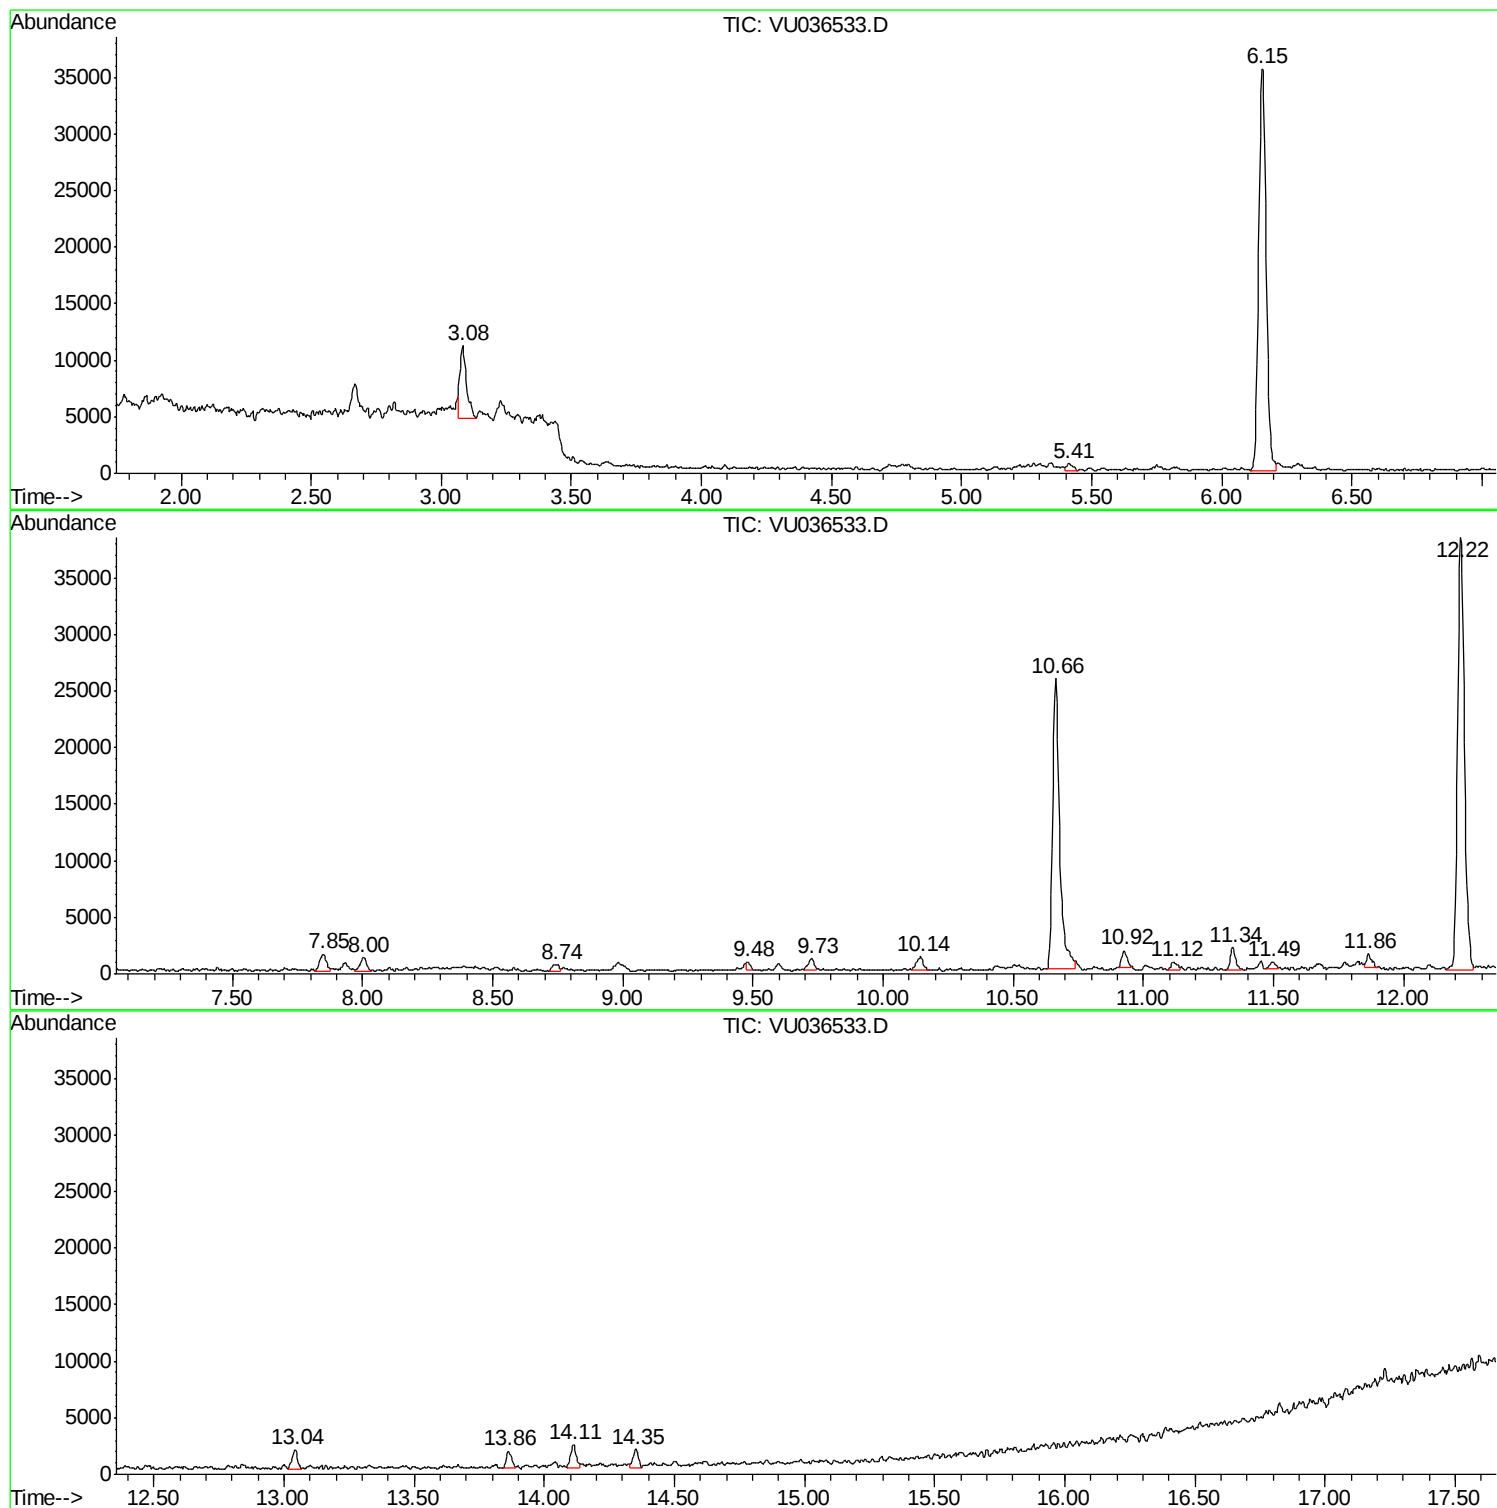

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036533.D
Acq On : 23 Jan 2020 11:00
Operator : JC/MD
Sample : VU0123WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0123WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036533.D
Acq On : 23 Jan 2020 11:00
Operator : JC/MD
Sample : VU0123WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0123WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc