

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036536.D
 Acq On : 23 Jan 2020 13:04
 Operator : JC/MD
 Sample : L1134-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-THM-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.735	1041	1056	1076	rBV2	7162	19967	1.36%	0.493%
2	5.134	1163	1180	1206	rBV	264876	570216	38.86%	14.070%
3	6.153	1483	1497	1512	rBV	37044	71203	4.85%	1.757%
4	7.144	1789	1805	1833	rBV	798390	1467488	100.00%	36.210%
5	8.841	2318	2333	2362	rBV	774898	1345679	91.70%	33.205%
6	10.317	2780	2792	2820	rBV	259810	449393	30.62%	11.089%
7	10.658	2887	2898	2919	rBV	32290	54461	3.71%	1.344%
8	12.217	3372	3383	3401	rVB2	42088	74261	5.06%	1.832%




Sum of corrected areas: 4052668

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036536.D
Acq On : 23 Jan 2020 13:04
Operator : JC/MD
Sample : L1134-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

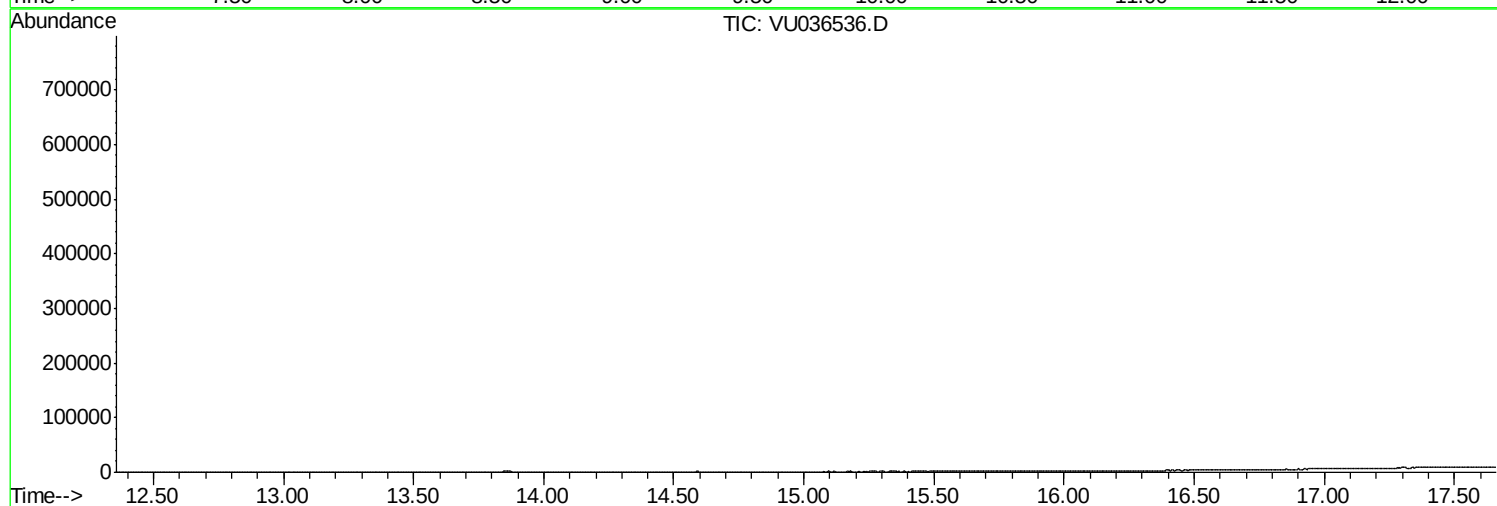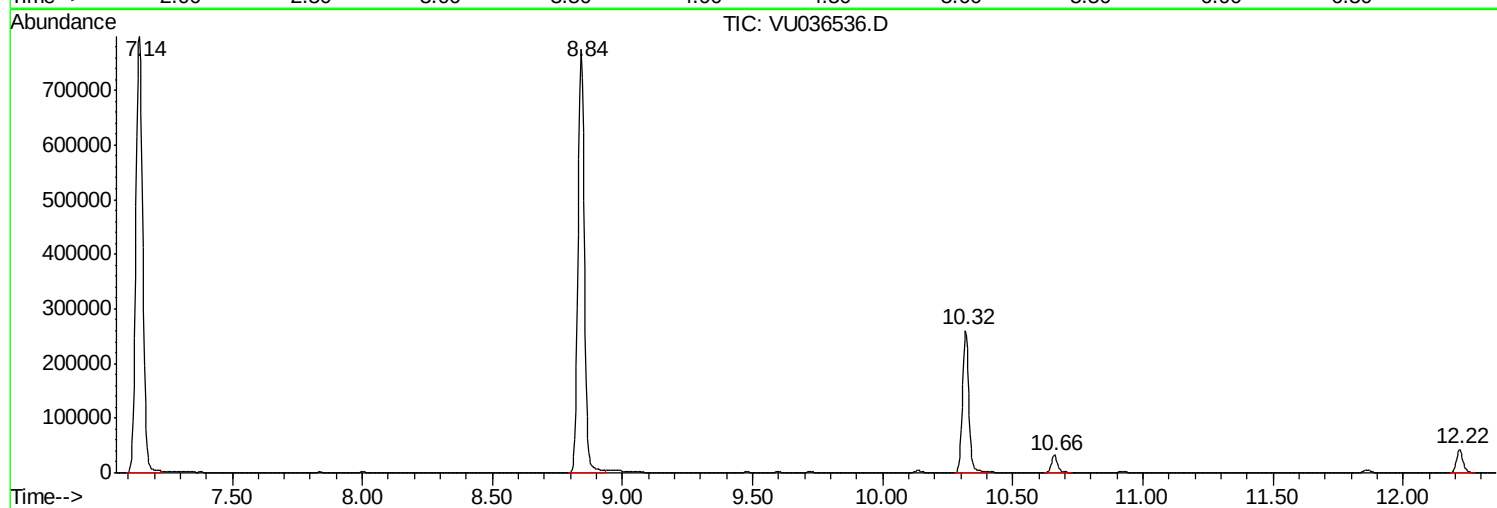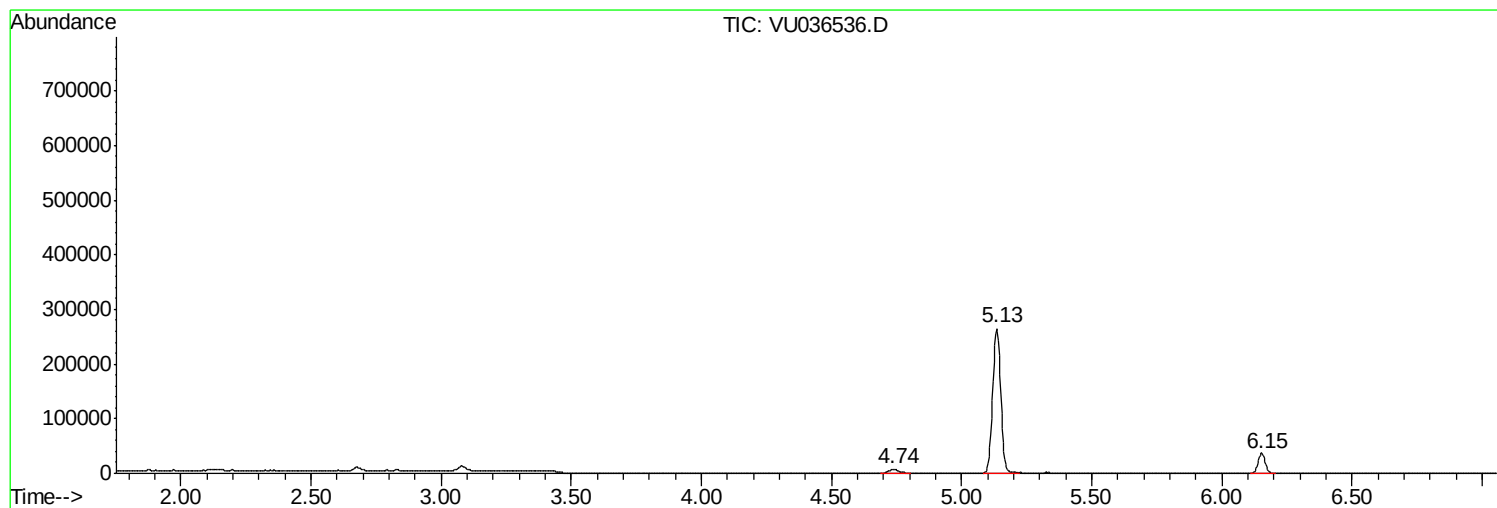

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036536.D
Acq On : 23 Jan 2020 13:04
Operator : JC/MD
Sample : L1134-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036536.D
Acq On : 23 Jan 2020 13:04
Operator : JC/MD
Sample : L1134-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc