

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036538.D
 Acq On : 23 Jan 2020 14:04
 Operator : JC/MD
 Sample : L1134-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.954	181	191	207	rBV	319143	416836	18.11%	1.567%
2	3.417	628	646	676	rVB	542965	1263857	54.91%	4.751%
3	3.915	782	801	820	rBV	117229	274122	11.91%	1.030%
4	4.710	1030	1048	1072	rBV	105565	267956	11.64%	1.007%
5	5.021	1129	1145	1167	rBV	71944	157303	6.83%	0.591%
6	5.565	1299	1314	1340	rBV	347054	703132	30.55%	2.643%
7	6.153	1479	1497	1514	rBV2	39079	76137	3.31%	0.286%
8	6.957	1732	1747	1764	rBV	60666	115880	5.03%	0.436%
9	7.642	1946	1960	1985	rBV	429947	752764	32.70%	2.830%
10	8.243	2134	2147	2182	rBV	369267	647993	28.15%	2.436%
11	8.607	2245	2260	2276	rBV	96357	172583	7.50%	0.649%
12	9.561	2545	2557	2577	rBV	175569	291469	12.66%	1.096%
13	10.507	2836	2851	2888	rBV	1101127	1728978	75.12%	6.500%
14	10.658	2888	2898	2914	rVB	38512	61114	2.66%	0.230%
15	10.806	2931	2944	2953	rBV2	663446	1090690	47.39%	4.100%
16	10.848	2953	2957	2970	rVV2	106078	162180	7.05%	0.610%
17	10.928	2970	2982	2996	rVV	1123811	1723126	74.86%	6.478%
18	11.008	2996	3007	3022	rVB	419065	678084	29.46%	2.549%
19	11.118	3027	3041	3071	rVB2	1285635	2295006	99.71%	8.627%
20	11.442	3127	3142	3150	rBV	1382078	2170478	94.30%	8.159%
21	11.487	3150	3156	3173	rVB	351272	529532	23.01%	1.991%
22	11.664	3193	3211	3230	rBV	1218977	1875652	81.49%	7.051%
23	11.767	3230	3243	3251	rVV	811448	1293685	56.20%	4.863%
24	11.812	3251	3257	3280	rVB	350916	531808	23.10%	1.999%
25	12.227	3371	3386	3408	rBV	1120929	1744504	75.79%	6.558%
26	14.037	3936	3949	3960	rBV	1477074	2301756	100.00%	8.653%
27	14.105	3960	3970	3989	rVB	953715	1531252	66.53%	5.756%
28	14.346	4032	4045	4062	rBV	1087183	1743807	75.76%	6.555%


Sum of corrected areas: 26601684

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036538.D
Acq On : 23 Jan 2020 14:04
Operator : JC/MD
Sample : L1134-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

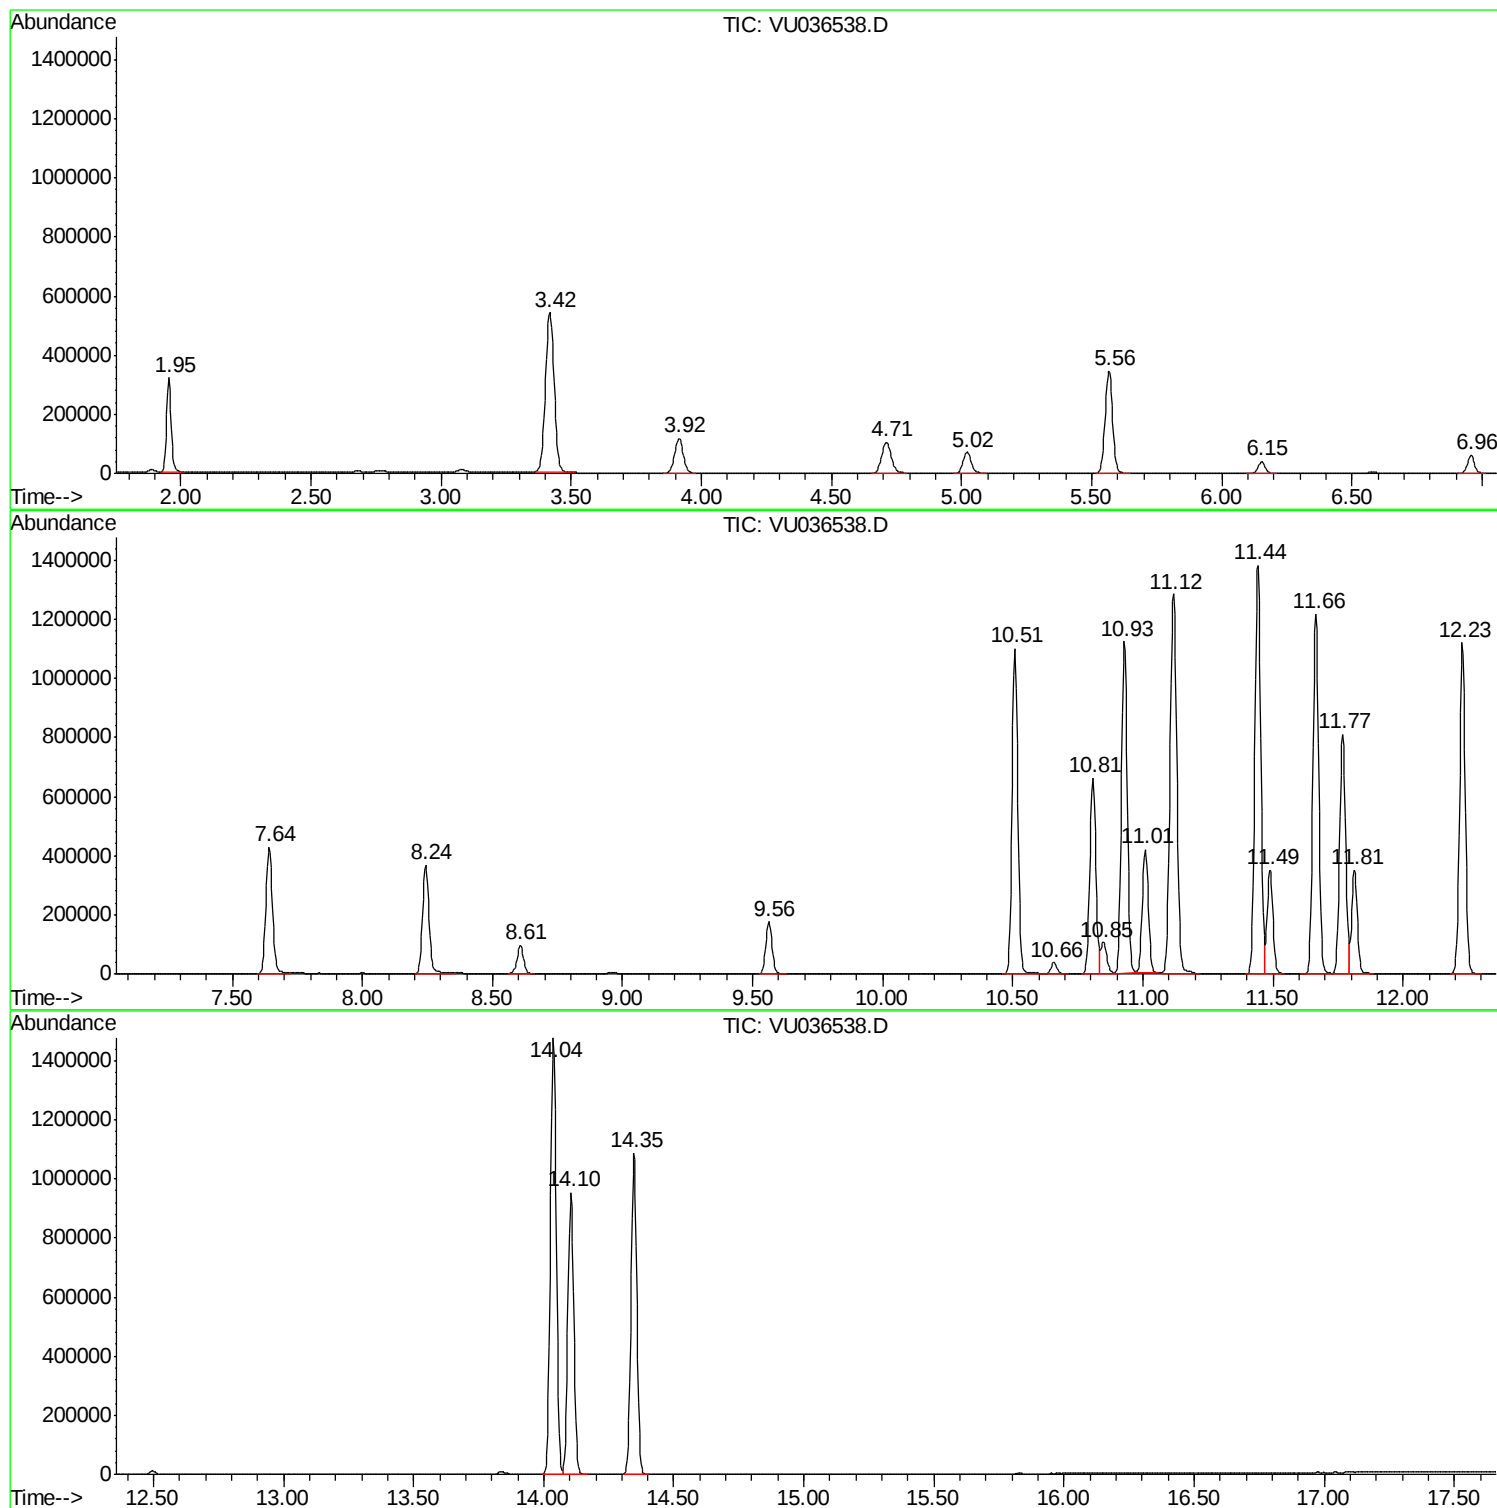

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036538.D
Acq On : 23 Jan 2020 14:04
Operator : JC/MD
Sample : L1134-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036538.D
Acq On : 23 Jan 2020 14:04
Operator : JC/MD
Sample : L1134-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc