

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036540.D
 Acq On : 23 Jan 2020 15:40
 Operator : JC/MD
 Sample : L1134-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-ADD-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.607	380	394	409	rBV	296558	544655	25.56%	7.336%
2	3.414	628	645	686	rVB	912075	2131093	100.00%	28.703%
3	4.054	822	844	873	rBV	324396	846754	39.73%	11.405%
4	4.562	981	1002	1028	rBV	519541	1302159	61.10%	17.538%
5	5.993	1429	1447	1476	rBV	466119	1000767	46.96%	13.479%
6	6.150	1483	1496	1514	rVB	38003	72591	3.41%	0.978%
7	10.658	2888	2898	2917	rBV	33183	56753	2.66%	0.764%
8	10.928	2967	2982	3014	rBV	873100	1388082	65.13%	18.695%
9	12.214	3371	3382	3398	rBV2	45981	81832	3.84%	1.102%


Sum of corrected areas: 7424686

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036540.D
Acq On : 23 Jan 2020 15:40
Operator : JC/MD
Sample : L1134-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

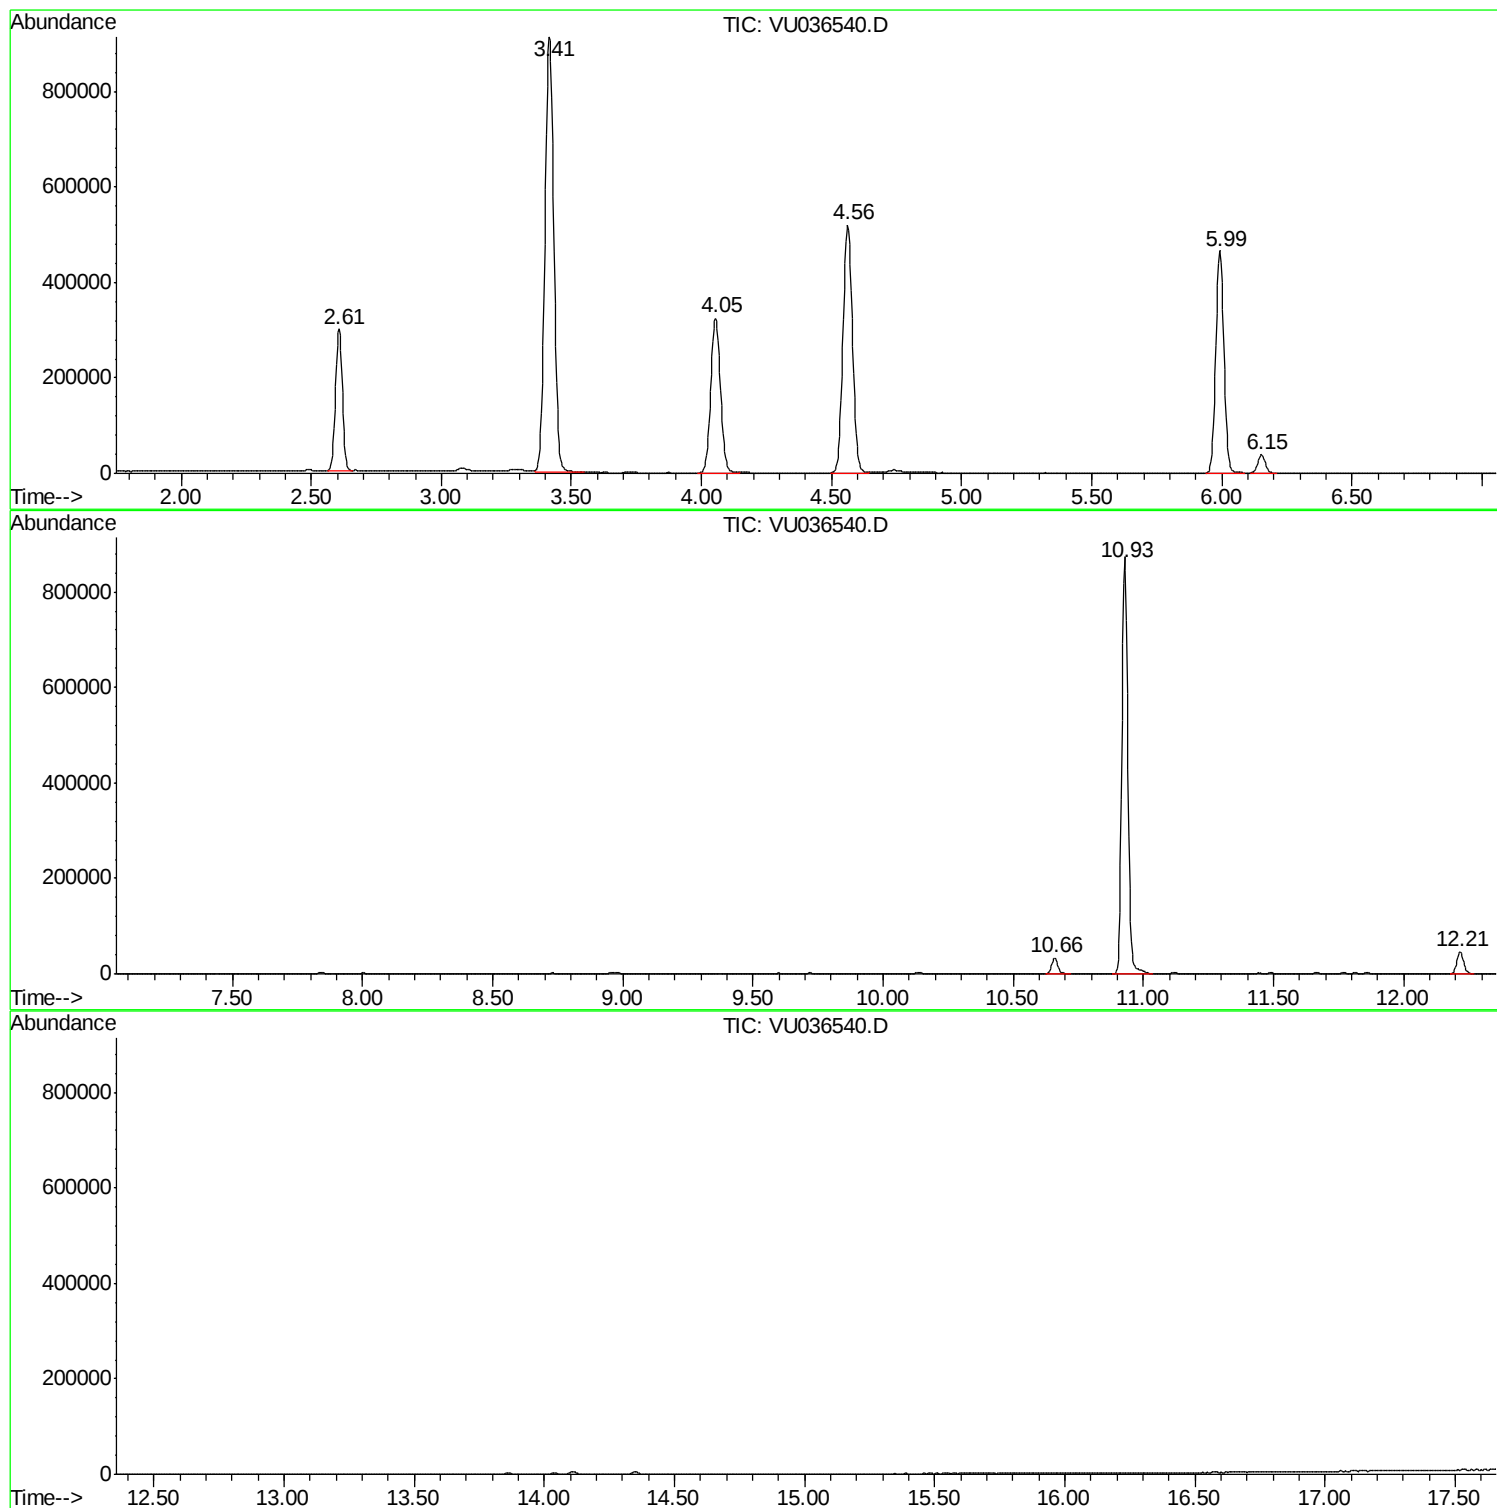

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036540.D
Acq On : 23 Jan 2020 15:40
Operator : JC/MD
Sample : L1134-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036540.D
Acq On : 23 Jan 2020 15:40
Operator : JC/MD
Sample : L1134-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc