

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012320\
 Data File : VU036541.D
 Acq On : 23 Jan 2020 16:07
 Operator : JC/MD
 Sample : L1134-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-EDBCP-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.083	534	542	554	rVB2	6342	12173	15.39%	3.319%
2	4.739	1039	1057	1082	rBV	8485	26630	33.67%	7.262%
3	6.153	1483	1497	1511	rBV	39212	75420	95.35%	20.566%
4	7.841	2015	2022	2028	rBV4	1607	2295	2.90%	0.626%
5	8.002	2062	2072	2080	rBV4	1575	2452	3.10%	0.669%
6	8.957	2359	2369	2392	rBV3	15019	31054	39.26%	8.468%
7	9.722	2597	2607	2615	rVB3	1081	1669	2.11%	0.455%
8	10.137	2726	2736	2745	rVB7	1750	2830	3.58%	0.772%
9	10.658	2888	2898	2922	rBV2	33954	59406	75.11%	16.199%
10	10.848	2948	2957	2969	rBV2	23383	38295	48.42%	10.443%
11	10.928	2969	2982	2996	rVB4	8377	14185	17.93%	3.868%
12	11.767	3238	3243	3252	rVB3	714	898	1.14%	0.245%
13	12.217	3371	3383	3401	rVB2	45772	79097	100.00%	21.569%
14	12.793	3551	3562	3569	rBV3	911	1463	1.85%	0.399%
15	13.021	3619	3633	3643	rBV2	8100	13188	16.67%	3.596%
16	14.037	3944	3949	3954	rBV4	849	997	1.26%	0.272%
17	14.108	3963	3971	3981	rBV	1663	2565	3.24%	0.699%
18	14.356	4040	4048	4053	rVB4	1534	2101	2.66%	0.573%


Sum of corrected areas: 366718

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036541.D
Acq On : 23 Jan 2020 16:07
Operator : JC/MD
Sample : L1134-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

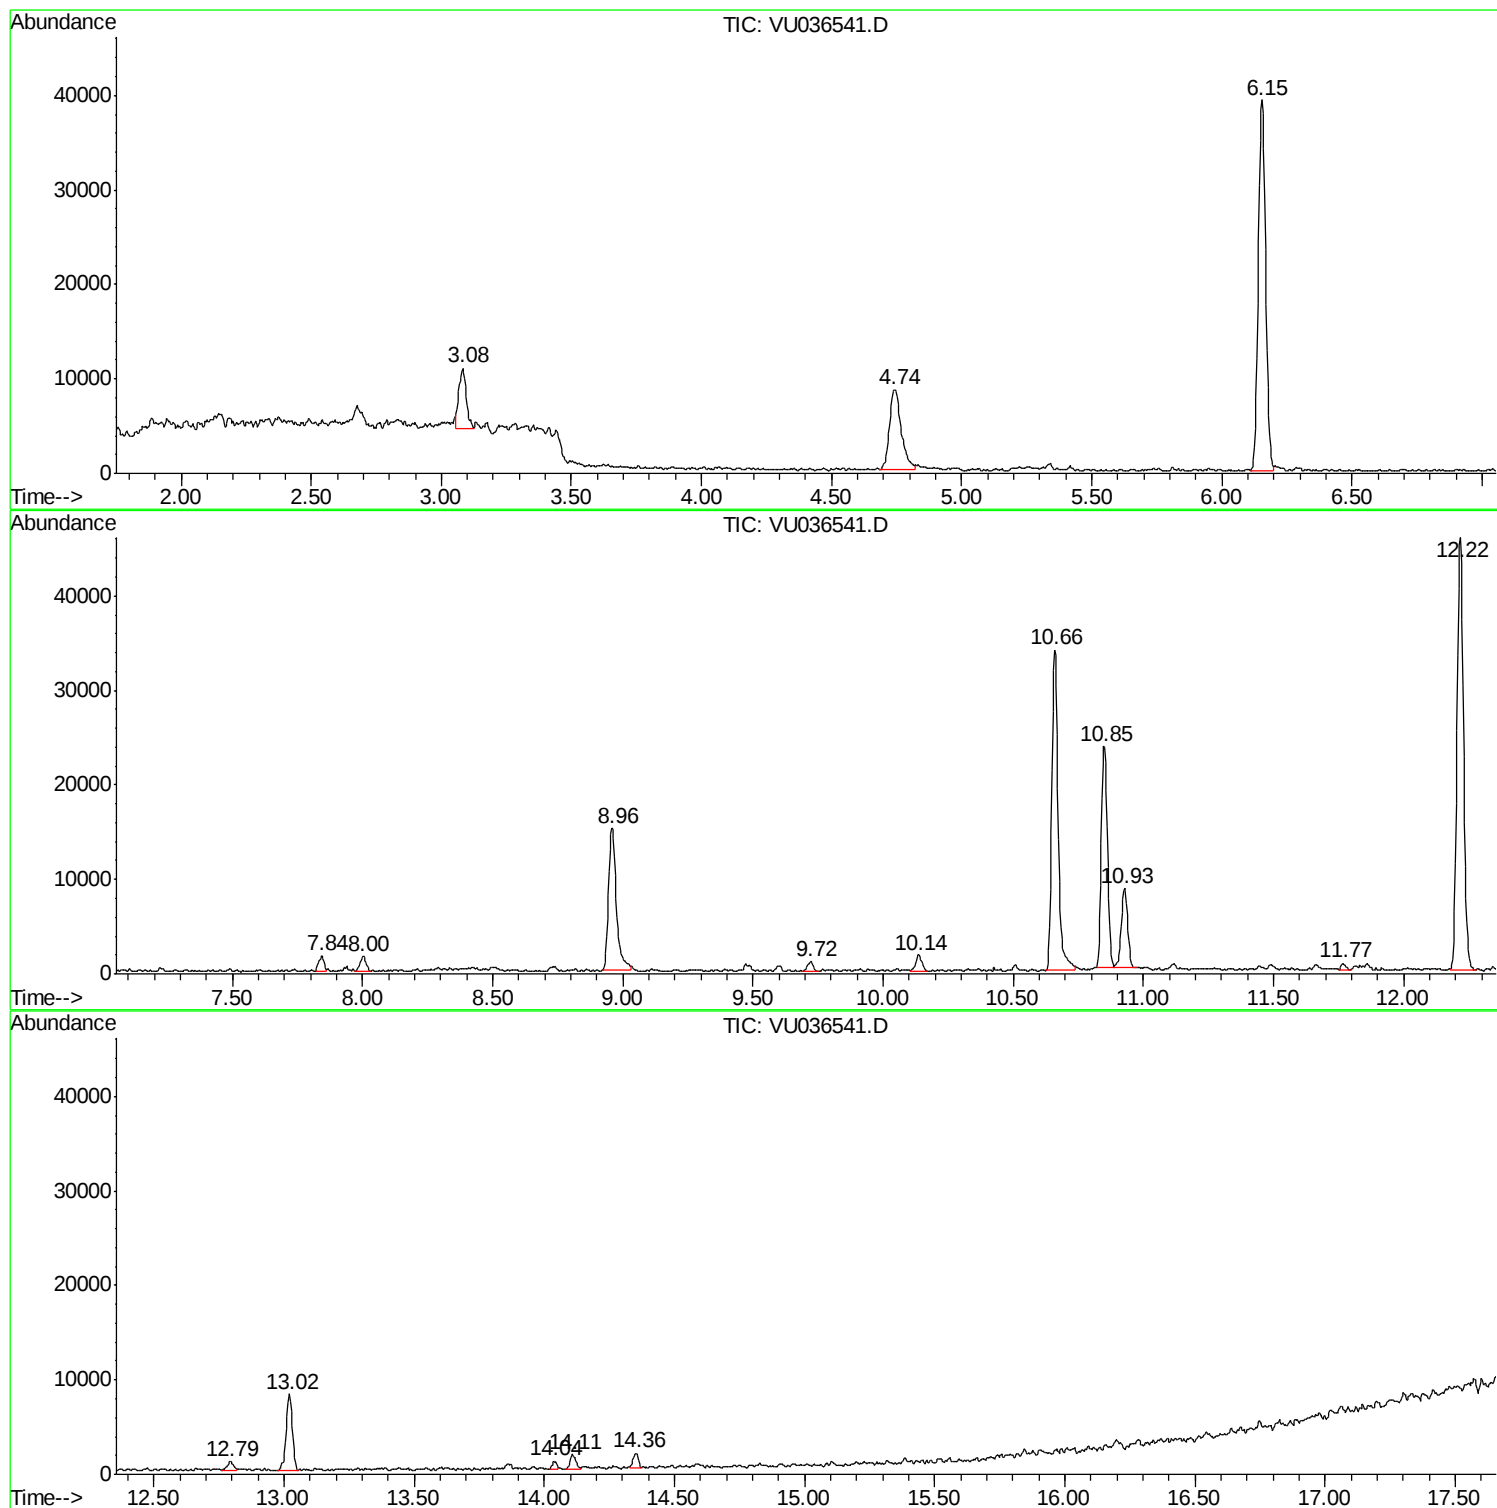

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU012320\
Data File : VU036541.D
Acq On : 23 Jan 2020 16:07
Operator : JC/MD
Sample : L1134-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, propyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.93	0.19 ug/l	14185	Fluorobenzene	6.15

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Benzene, propyl-	120	C9H12	000103-65-1	46
2		Benzene, propyl-	120	C9H12	000103-65-1	46
3		Benzene, propyl-	120	C9H12	000103-65-1	46
4		N-Benzyl-2-phenethylamine	211	C15H17N	003647-71-0	43
5		1,3,5-Cycloheptatriene, 7-ethyl-	120	C9H12	017634-51-4	37

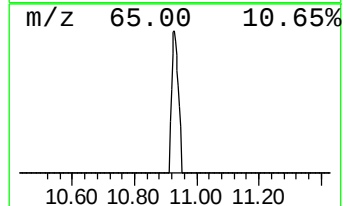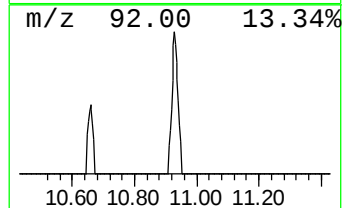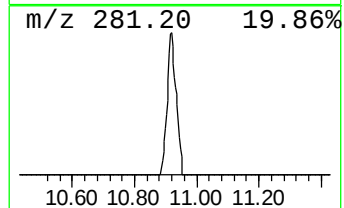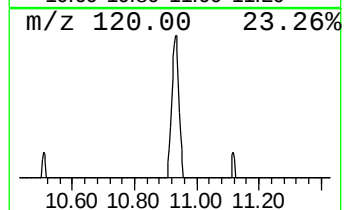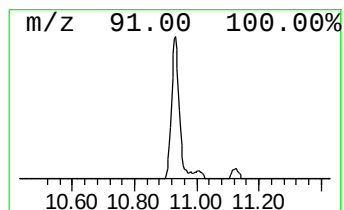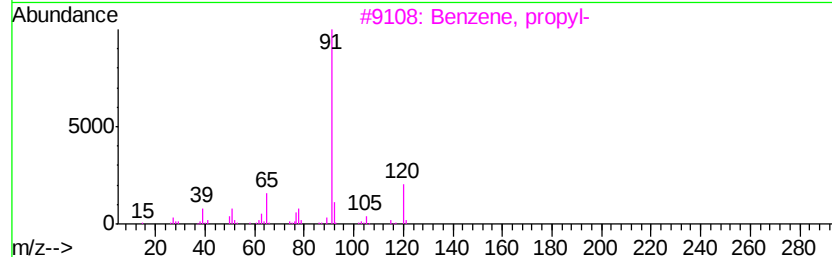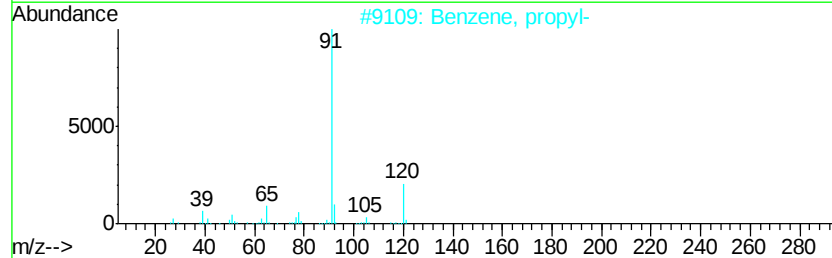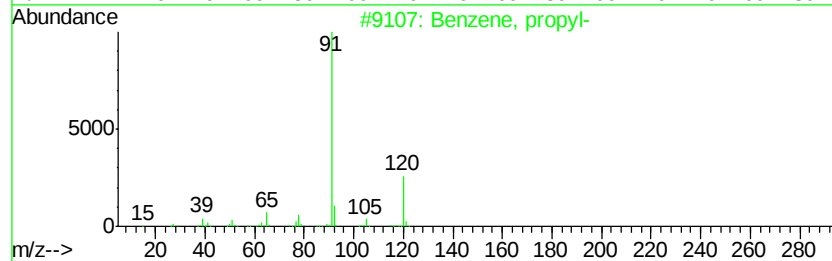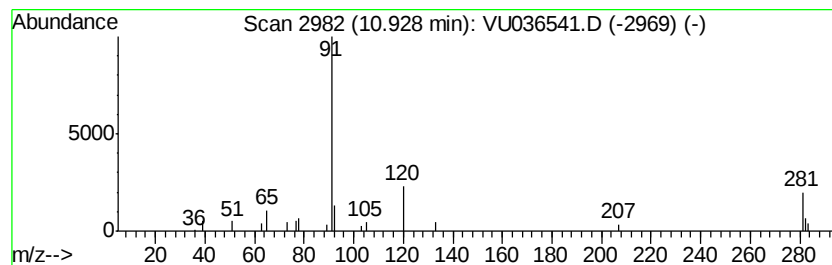

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU012320\
Data File : VU036541.D
Acq On : 23 Jan 2020 16:07
Operator : JC/MD
Sample : L1134-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-EDBCP-WS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, propyl-	10.93	0.2	ug/l	14185	1	6.15	75420	1.0