


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU012320\
 Data File : VU036531.D
 Acq On : 23 Jan 2020 09:27
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012220DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jan 23 08:59:25 2020

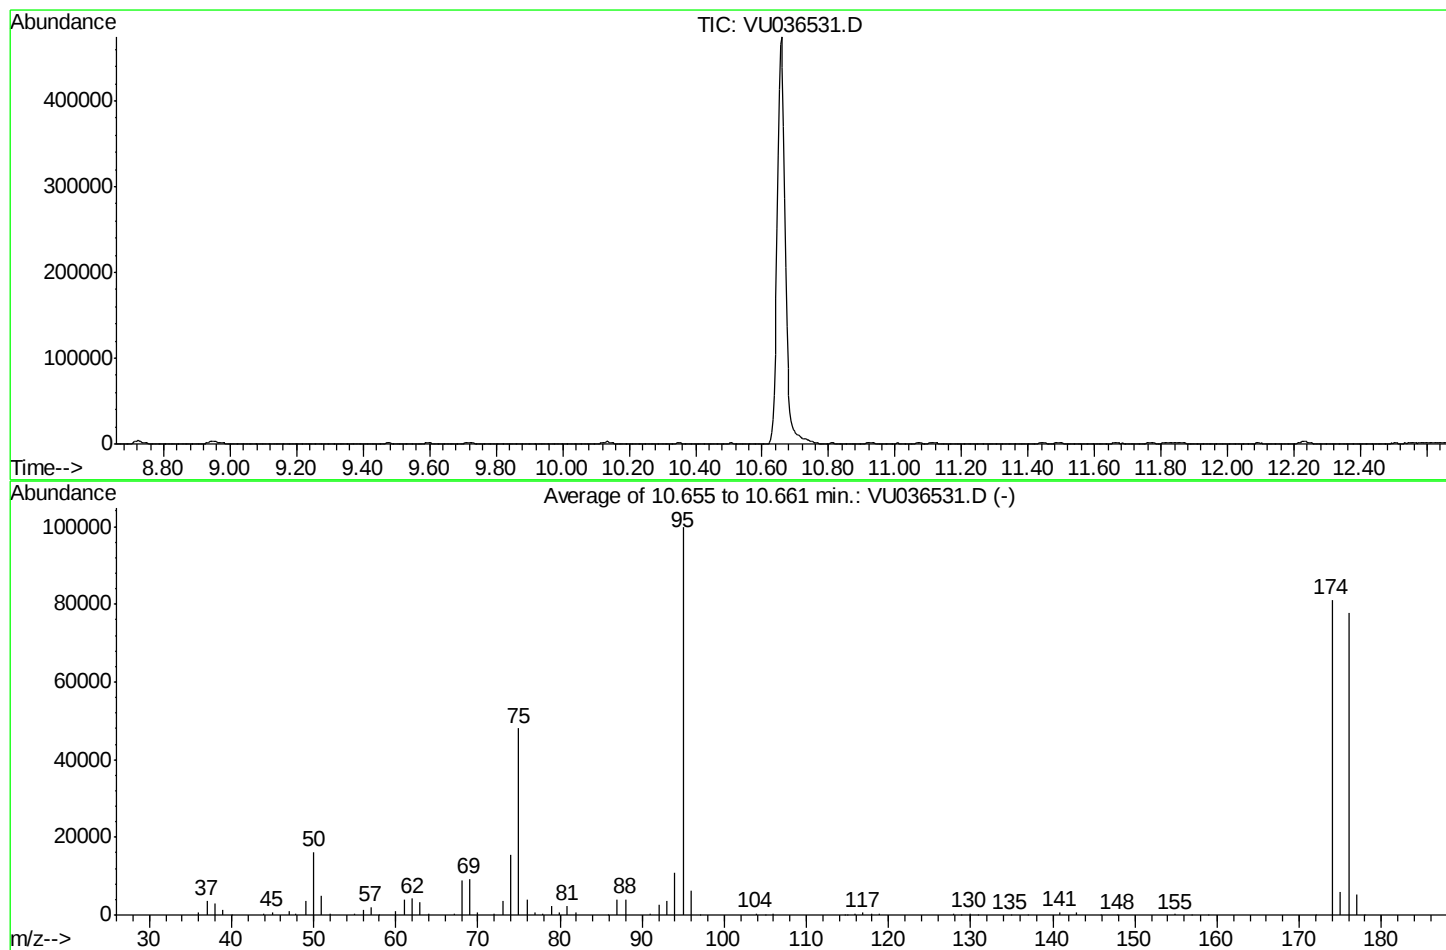

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	16285	PASS
75	95	30	60	48.1	47976	PASS
95	95	100	100	100.0	99800	PASS
96	95	5	9	6.4	6433	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.2	81082	PASS
175	174	5	9	7.5	6090	PASS
176	174	95	101	95.9	77762	PASS
177	176	5	9	6.6	5126	PASS