


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012323\
Data File : VU052770.D
Acq On : 23 Jan 2023 10:19
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jan 24 05:16:59 2023

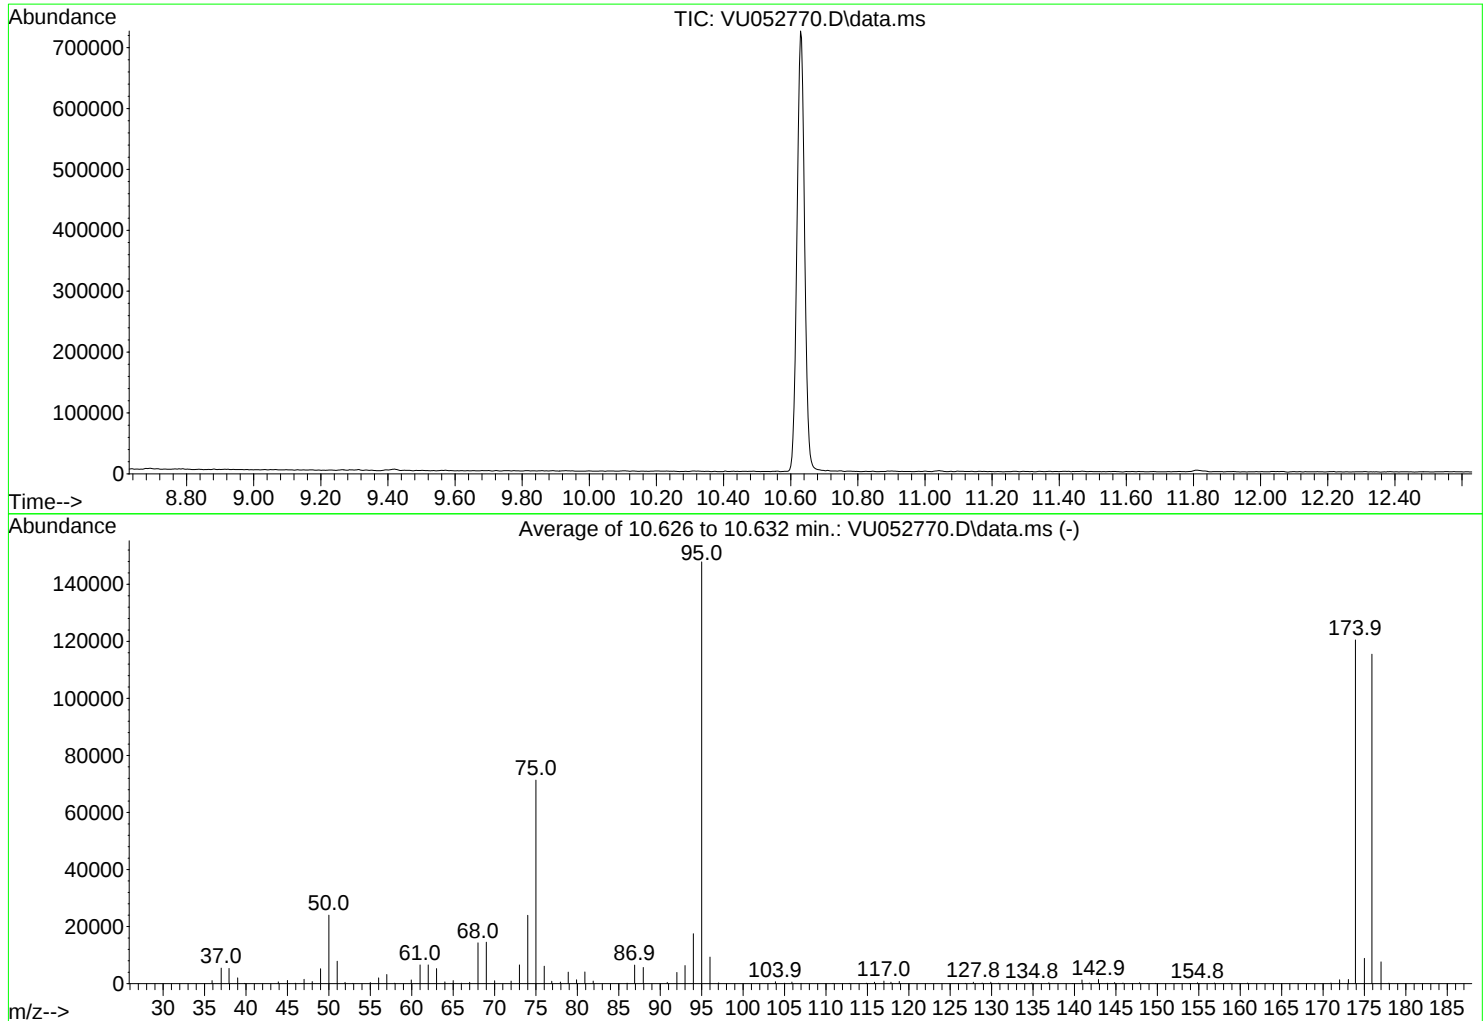

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	24011	PASS
75	95	30	60	48.2	71339	PASS
95	95	100	100	100.0	147883	PASS
96	95	5	9	6.3	9303	PASS
173	174	0.00	2	1.2	1486	PASS
174	95	50	100	81.5	120520	PASS
175	174	5	9	7.4	8863	PASS
176	174	95	101	95.8	115483	PASS
177	176	5	9	6.6	7608	PASS