

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
 Data File : VU057583.D
 Acq On : 23 Jan 2024 21:33
 Operator : MD/SY
 Sample : P1228-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B98

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	86	96	108	rVB	25793	31138	16.26%	1.851%
2	1.914	185	194	209	rBV	19607	26547	13.87%	1.578%
3	2.566	385	397	414	rVB	42690	71256	37.22%	4.236%
4	3.177	575	587	600	rBV2	2877	6512	3.40%	0.387%
5	3.293	600	623	627	rBV3	3202	9967	5.21%	0.593%
6	4.640	1026	1042	1085	rBV2	21676	73490	38.38%	4.369%
7	5.055	1157	1171	1195	rVB	36673	81307	42.47%	4.834%
8	5.721	1360	1378	1404	rBV2	75210	191455	100.00%	11.382%
9	6.245	1528	1541	1571	rBV	74723	146276	76.40%	8.696%
10	6.685	1663	1678	1699	rBV	45290	88014	45.97%	5.233%
11	7.563	1941	1951	1970	rBV2	23926	42650	22.28%	2.536%
12	7.894	2042	2054	2074	rBV	95668	173060	90.39%	10.289%
13	8.177	2132	2142	2157	rBV2	12486	22356	11.68%	1.329%
14	8.550	2248	2258	2268	rBV	12675	20983	10.96%	1.247%
15	8.634	2272	2284	2312	rBV3	71813	166149	86.78%	9.878%
16	9.412	2515	2526	2549	rBV	101439	175226	91.52%	10.417%
17	10.749	2931	2942	2960	rBV2	27658	44766	23.38%	2.661%
18	11.807	3260	3271	3300	rVB	106743	173004	90.36%	10.285%
19	12.187	3378	3389	3414	rBV	78410	130983	68.41%	7.787%
20	12.762	3560	3568	3579	rBB2	4434	6917	3.61%	0.411%




Sum of corrected areas: 1682056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057583.D
Acq On : 23 Jan 2024 21:33
Operator : MD/SY
Sample : P1228-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

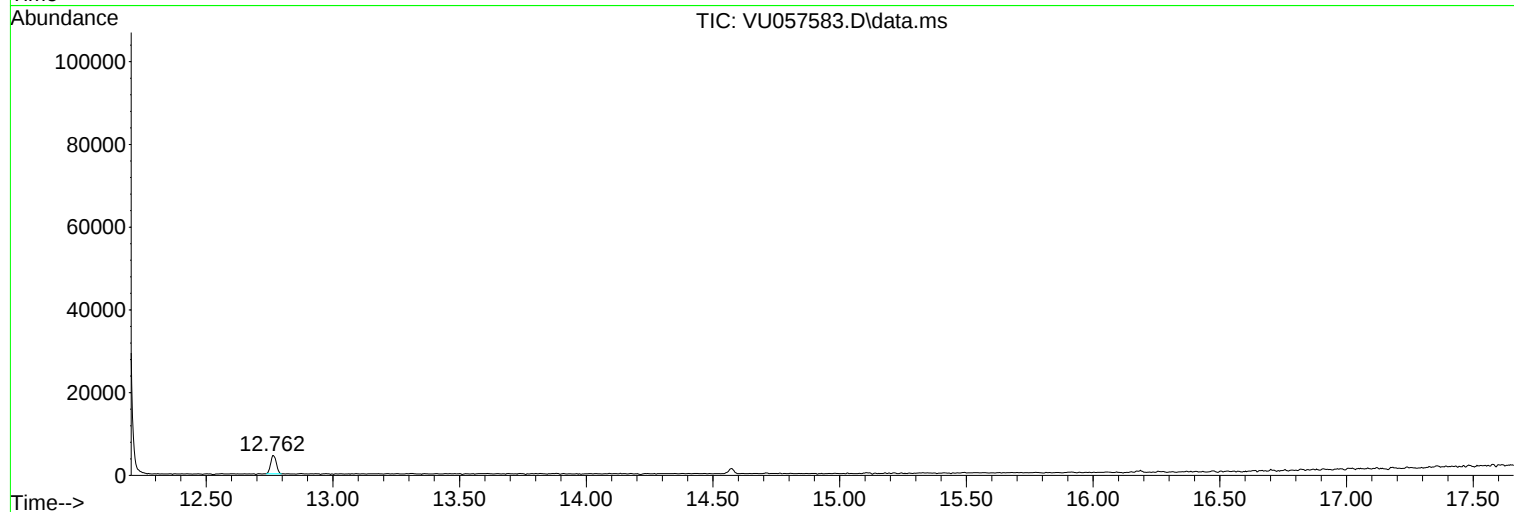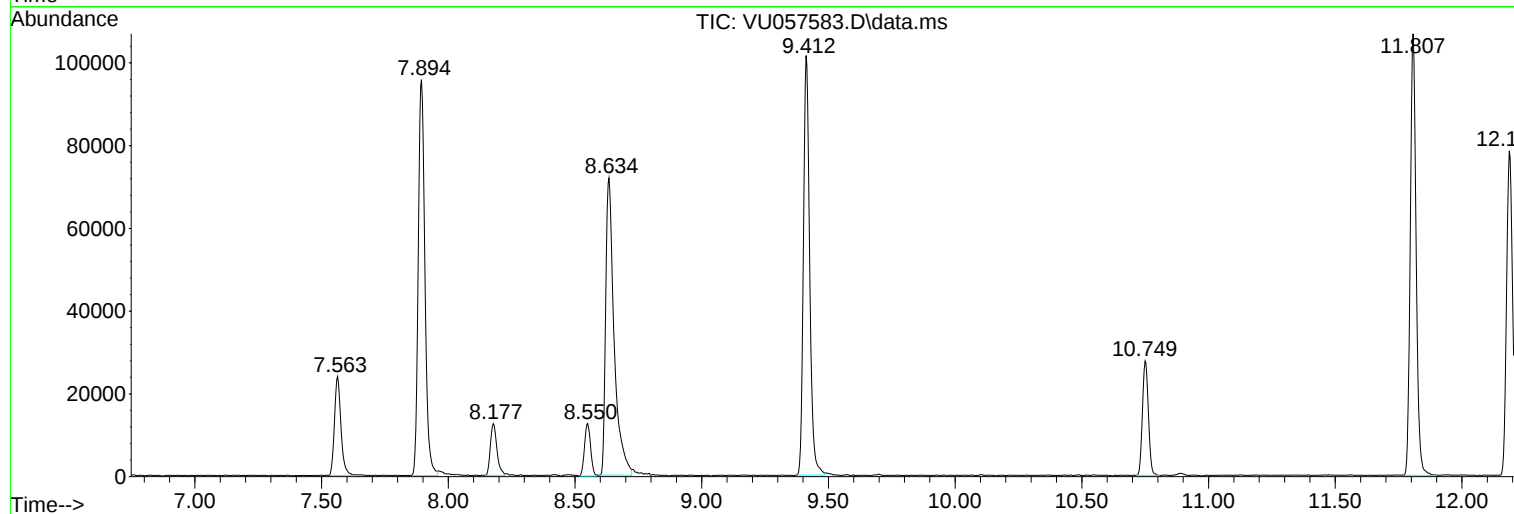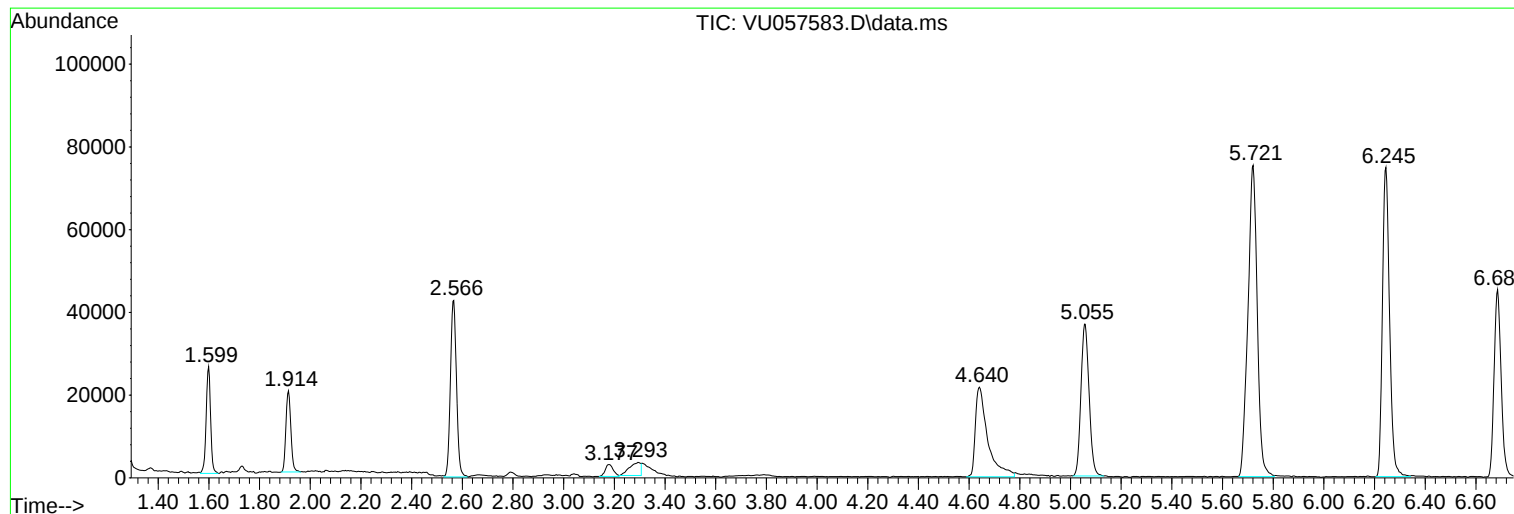

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057583.D
Acq On : 23 Jan 2024 21:33
Operator : MD/SY
Sample : P1228-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057583.D
Acq On : 23 Jan 2024 21:33
Operator : MD/SY
Sample : P1228-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc