

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
 Data File : VU057594.D
 Acq On : 24 Jan 2024 02:23
 Operator : MD/SY
 Sample : VU0123WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK133

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	109	rVB	23650	27338	15.51%	1.786%
2	1.914	186	194	207	rVB	18915	24784	14.06%	1.619%
3	2.563	384	396	412	rVB	39889	65889	37.37%	4.305%
4	3.043	535	545	559	rVB3	2650	4779	2.71%	0.312%
5	4.641	1024	1042	1072	rBV	16895	53429	30.30%	3.491%
6	5.055	1157	1171	1192	rBV	34392	76525	43.40%	5.000%
7	5.721	1359	1378	1403	rBV2	70136	176315	100.00%	11.521%
8	6.245	1529	1541	1570	rBV	74467	145263	82.39%	9.492%
9	6.685	1666	1678	1700	rVB2	41685	81671	46.32%	5.337%
10	7.563	1939	1951	1970	rBV2	20989	38026	21.57%	2.485%
11	7.894	2041	2054	2074	rBV	89740	159794	90.63%	10.441%
12	8.177	2133	2142	2166	rBV2	11324	20655	11.71%	1.350%
13	8.634	2272	2284	2321	rBV3	65241	149312	84.68%	9.756%
14	9.412	2515	2526	2561	rBV	99631	175071	99.29%	11.440%
15	10.750	2932	2942	2958	rVB	24938	40127	22.76%	2.622%
16	11.807	3260	3271	3291	rBV	97099	160269	90.90%	10.472%
17	12.187	3378	3389	3411	rBV	68129	115501	65.51%	7.547%
18	12.766	3559	3569	3579	rVB	4012	5742	3.26%	0.375%
19	13.843	3898	3904	3914	rBV3	1843	2654	1.51%	0.173%
20	14.100	3977	3984	3999	rBV	764	1943	1.10%	0.127%
21	14.325	4049	4054	4067	rVB3	1599	2368	1.34%	0.155%
22	14.569	4121	4130	4138	rBV	1770	2933	1.66%	0.192%




Sum of corrected areas: 1530388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057594.D
Acq On : 24 Jan 2024 02:23
Operator : MD/SY
Sample : VU0123WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

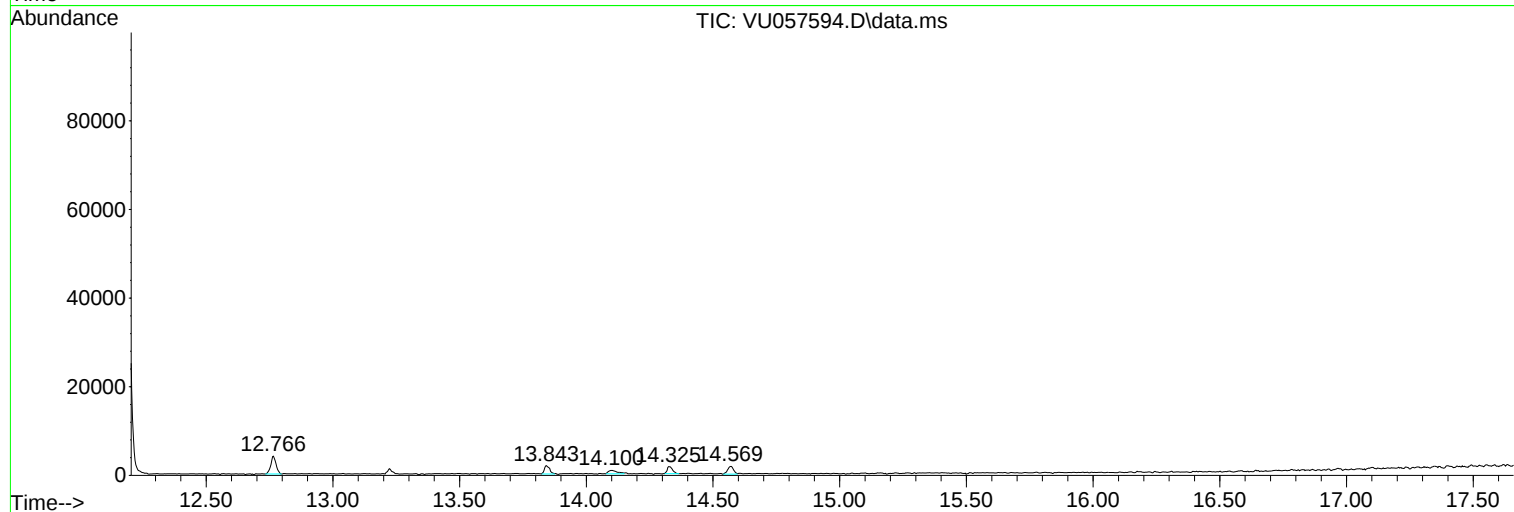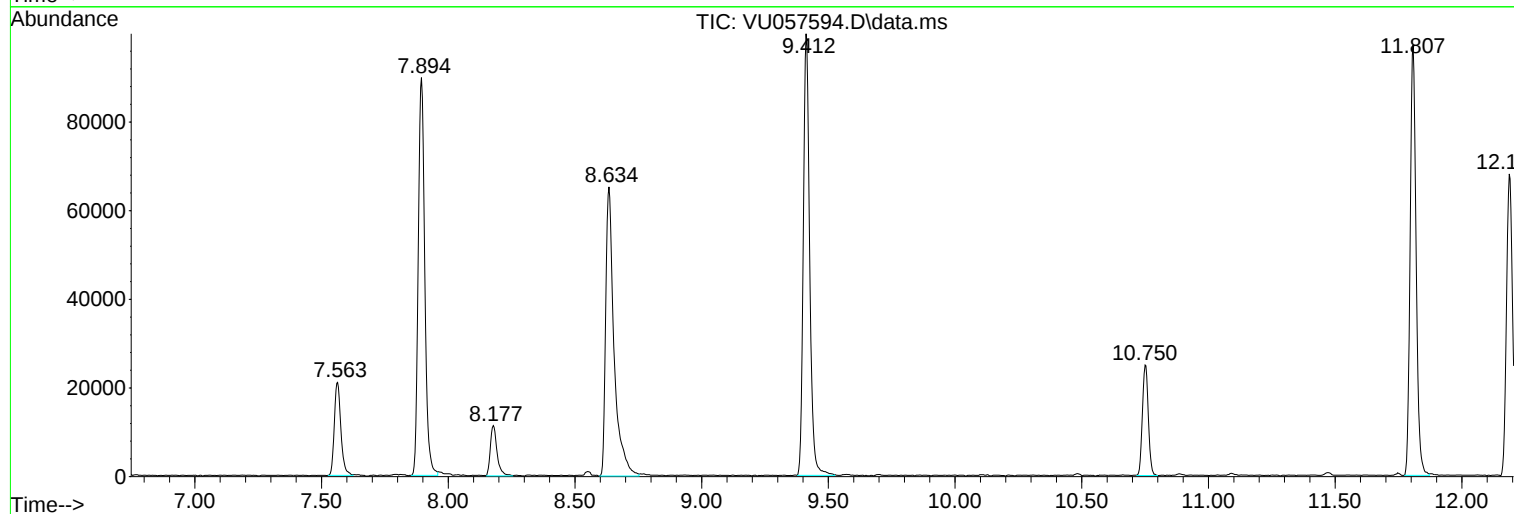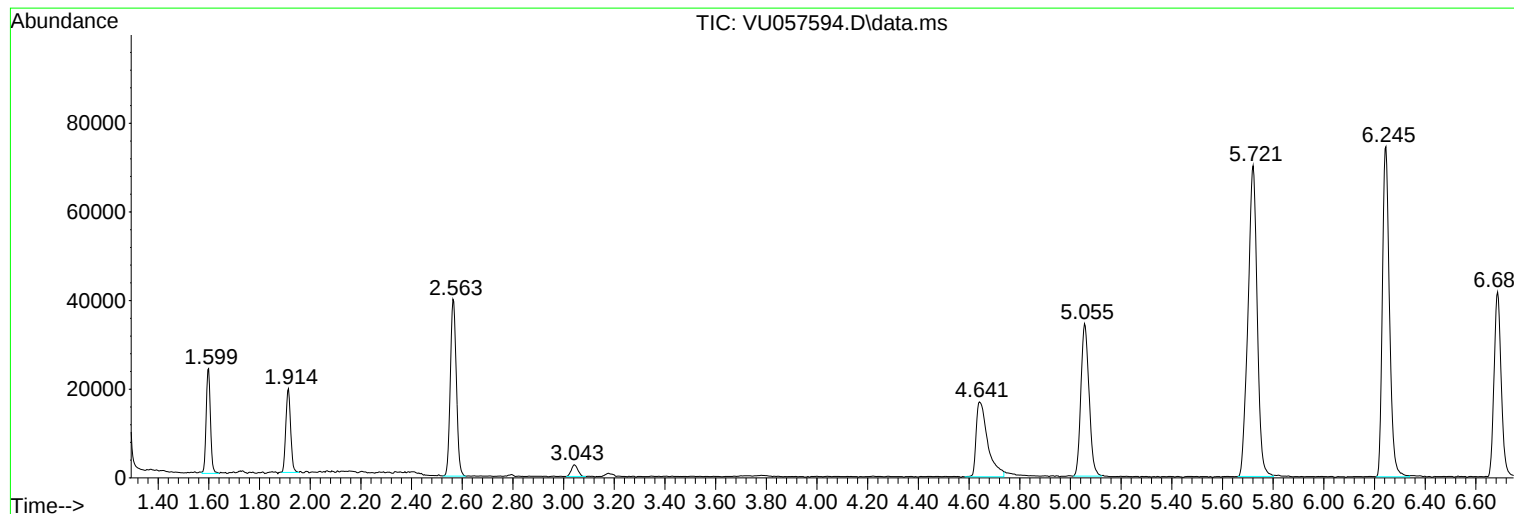

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057594.D
Acq On : 24 Jan 2024 02:23
Operator : MD/SY
Sample : VU0123WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057594.D
Acq On : 24 Jan 2024 02:23
Operator : MD/SY
Sample : VU0123WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc