

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
 Data File : VU057607.D
 Acq On : 24 Jan 2024 07:37
 Operator : MD/SY
 Sample : P1227-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B94

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	107	rVB	22548	26657	15.35%	1.645%
2	1.730	131	137	145	rVB	2811	3372	1.94%	0.208%
3	1.914	184	194	206	rBV	17929	23741	13.67%	1.465%
4	2.563	385	396	413	rVB	38882	63197	36.39%	3.899%
5	3.181	576	588	601	rBV2	3866	8557	4.93%	0.528%
6	3.293	608	623	627	rBV5	1977	4928	2.84%	0.304%
7	4.644	1026	1043	1089	rBV3	20827	72411	41.70%	4.468%
8	5.055	1157	1171	1199	rVB	33682	75159	43.28%	4.637%
9	5.721	1357	1378	1401	rBV2	68421	173650	100.00%	10.714%
10	6.245	1529	1541	1563	rBV	71344	137893	79.41%	8.508%
11	6.685	1663	1678	1699	rBV	40047	78886	45.43%	4.867%
12	7.563	1938	1951	1970	rBV	20752	37485	21.59%	2.313%
13	7.894	2042	2054	2080	rBV	87000	155358	89.47%	9.585%
14	8.177	2133	2142	2156	rBV2	10771	18874	10.87%	1.164%
15	8.547	2246	2257	2273	rBV	59437	101491	58.45%	6.262%
16	8.634	2273	2284	2315	rBV3	64722	147903	85.17%	9.125%
17	9.412	2514	2526	2563	rBV	97556	168053	96.78%	10.368%
18	10.749	2932	2942	2955	rBV	24628	40326	23.22%	2.488%
19	11.807	3259	3271	3297	rBV	99190	160385	92.36%	9.895%
20	12.187	3377	3389	3406	rBV	71536	117861	67.87%	7.272%
21	12.765	3558	3569	3579	rBV2	2937	4630	2.67%	0.286%




Sum of corrected areas: 1620817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057607.D
Acq On : 24 Jan 2024 07:37
Operator : MD/SY
Sample : P1227-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

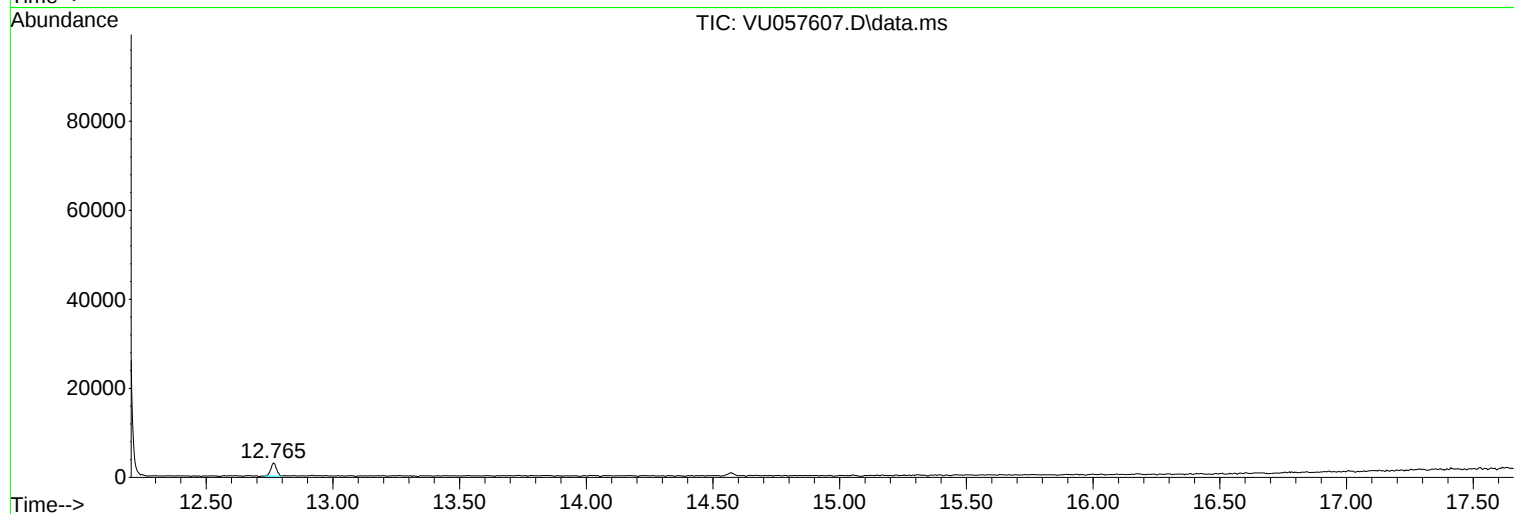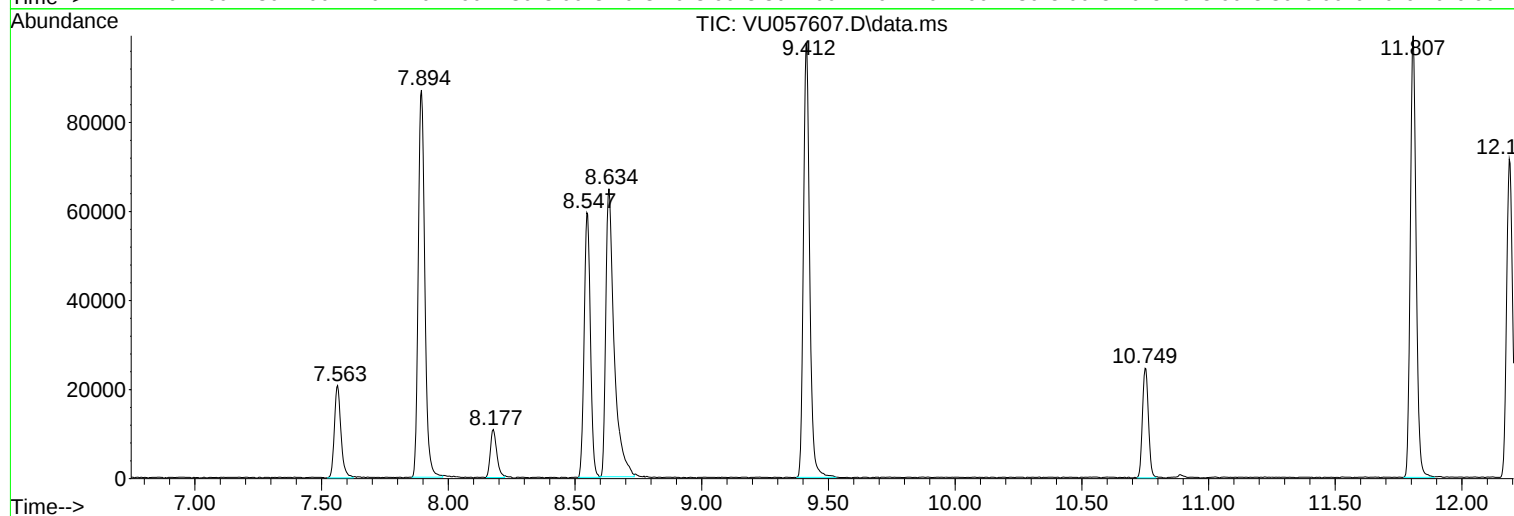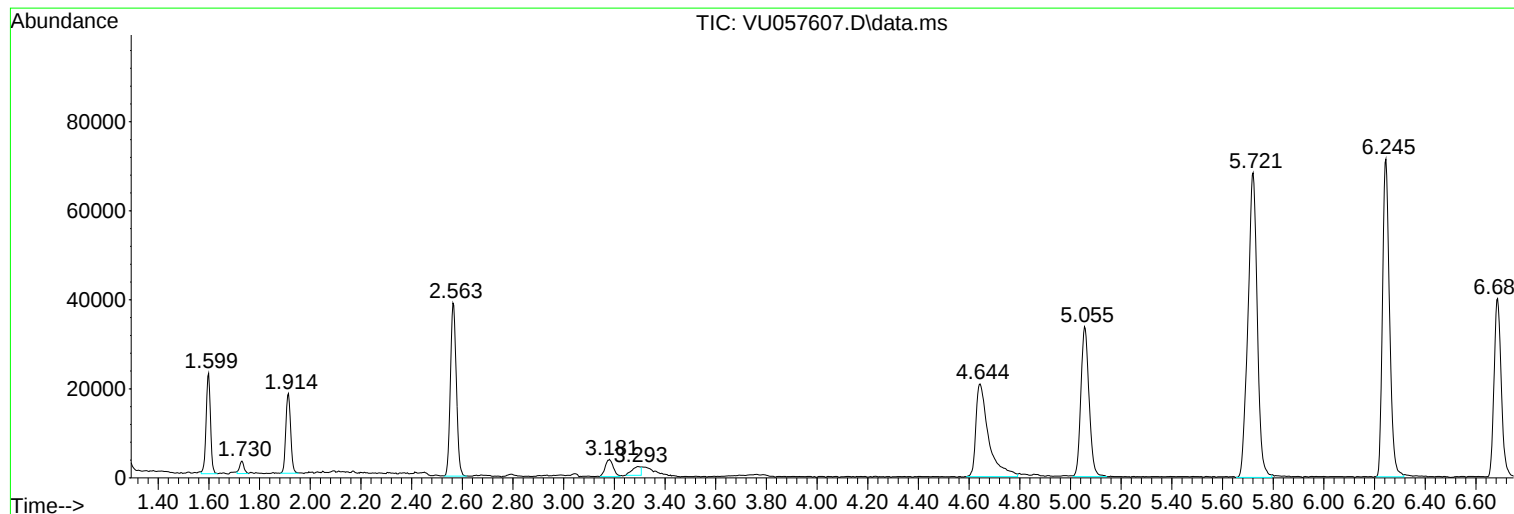

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057607.D
Acq On : 24 Jan 2024 07:37
Operator : MD/SY
Sample : P1227-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057607.D
Acq On : 24 Jan 2024 07:37
Operator : MD/SY
Sample : P1227-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc