


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012324\
Data File : VU057564.D
Acq On : 23 Jan 2024 09:56
Operator : MD/SY
Sample : BFB109
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB109

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 00:30:52 2024

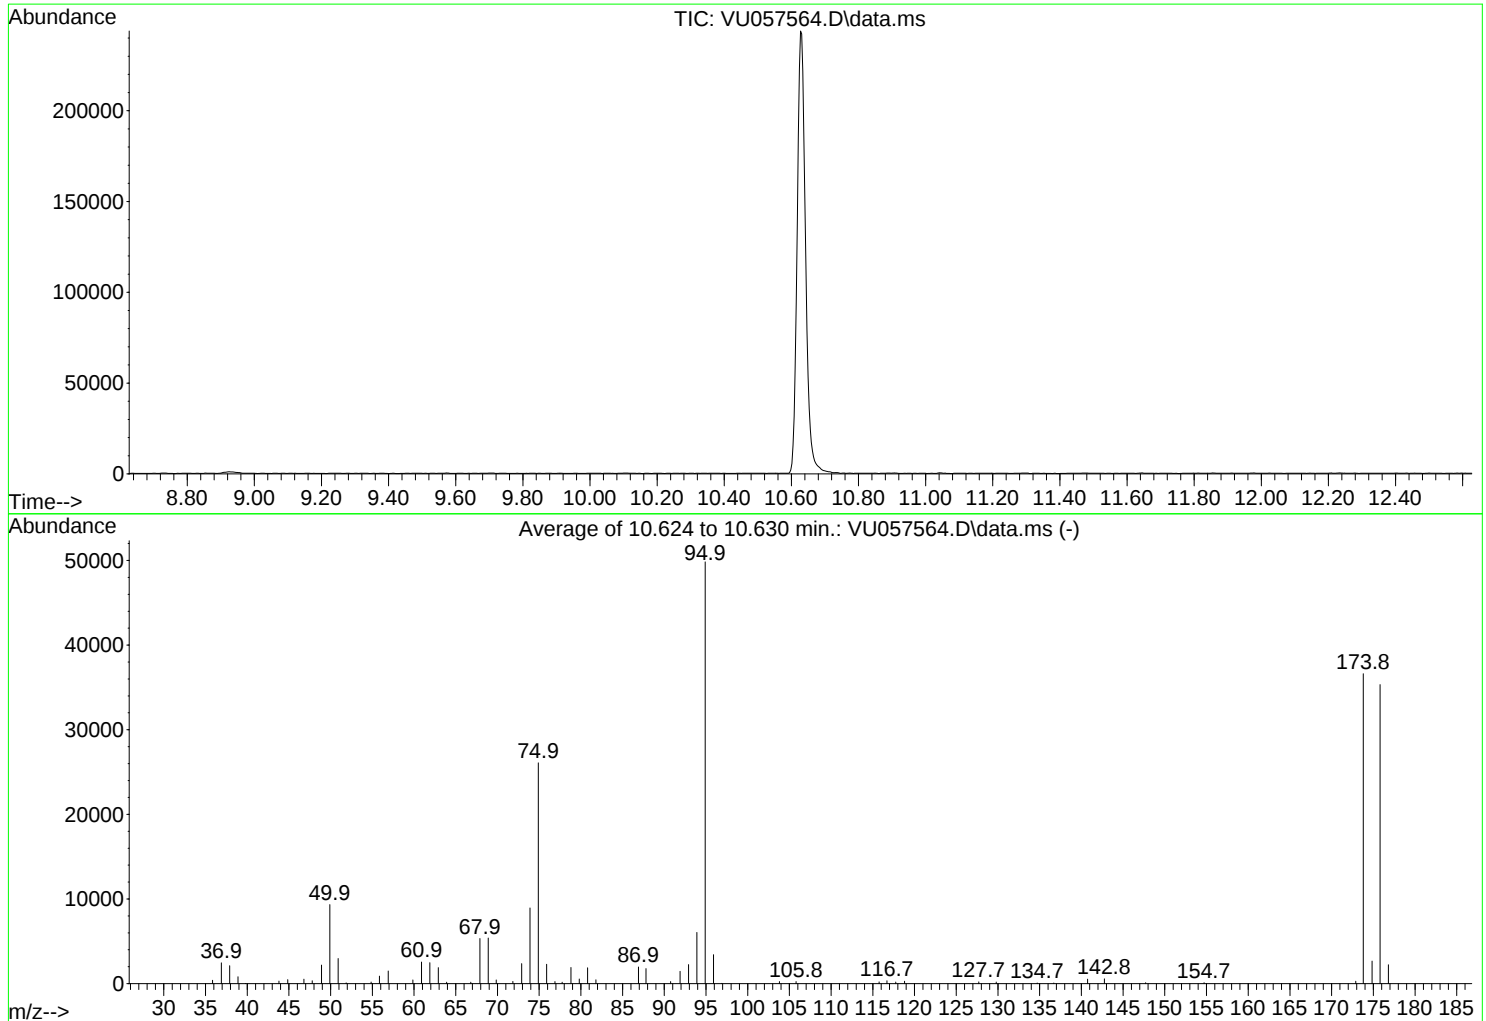

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9348	PASS
75	95	30	80	52.3	26088	PASS
95	95	100	100	100.0	49837	PASS
96	95	5	9	6.9	3429	PASS
173	174	0.00	2	0.8	286	PASS
174	95	50	120	73.5	36613	PASS
175	174	5	9	7.3	2665	PASS
176	174	95	101	96.5	35341	PASS
177	176	5	9	6.3	2239	PASS

m/z	Abundance
39.80	155.0
43.80	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.90	339.0
36.90	2378.0
37.90	2009.0
38.90	771.0
39.80	174.0
43.80	537.0
44.90	435.0
46.80	522.0
47.80	305.0
48.90	2127.0
49.90	9096.0
50.90	2847.0
51.80	101.0
54.80	183.0
55.80	889.0
56.90	1442.0
59.80	434.0
60.90	2510.0
61.90	2408.0
62.90	1833.0
63.90	149.0
66.80	161.0
67.90	5073.0
68.90	5169.0
69.80	424.0
71.90	237.0
72.90	2243.0
73.90	8468.0
74.90	24872.0
75.90	2206.0
76.90	236.0
77.70	161.0
78.80	1799.0
79.80	527.0
80.80	1748.0
81.80	443.0
86.90	1835.0
87.80	1668.0
90.80	237.0
91.90	1392.0
92.90	2119.0
93.90	5718.0
94.90	47384.0
95.90	3390.0
103.80	238.0
105.80	225.0
115.70	188.0
116.70	332.0
117.70	194.0
118.80	262.0
127.70	184.0
129.80	180.0
140.70	511.0
142.70	508.0
147.70	110.0
154.70	108.0
172.90	289.0
173.80	33952.0
174.90	2548.0
175.80	32728.0
176.80	2071.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.80	401.0
36.90	2542.0
37.90	2189.0
38.90	839.0
39.80	165.0
43.90	525.0
44.80	474.0
46.80	544.0
47.80	364.0
48.90	2267.0
49.90	9614.0
50.90	3054.0
51.90	107.0
54.90	186.0
55.80	920.0
56.90	1552.0
59.90	451.0
60.90	2640.0
61.90	2545.0
62.90	1949.0
63.90	177.0
66.80	181.0
67.90	5498.0
68.90	5557.0
69.90	439.0
71.80	276.0
72.90	2447.0
73.90	9252.0
74.90	26840.0
75.90	2330.0
76.90	256.0
77.70	182.0
78.80	1954.0
79.80	567.0
80.80	1929.0
81.80	467.0
86.90	2048.0
87.80	1833.0
90.70	255.0
91.90	1488.0
92.90	2346.0
93.90	6226.0
94.90	51392.0
95.90	3540.0
103.80	248.0
105.80	242.0
115.80	211.0
116.70	346.0
117.80	206.0
118.80	292.0
127.70	216.0
129.80	187.0
134.70	109.0
136.70	109.0
140.70	552.0
142.80	588.0
147.70	120.0
154.70	117.0
172.90	284.0
173.80	37704.0
174.80	2740.0
175.80	36488.0
176.80	2308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109

m/z	Abundance
35.80	430.0
36.90	2468.0
37.90	2158.0
38.90	842.0
39.80	166.0
43.90	474.0
44.80	485.0
46.80	500.0
47.80	379.0
48.90	2199.0
49.90	9334.0
50.90	3032.0
51.90	107.0
54.90	178.0
55.90	845.0
56.90	1511.0
59.90	451.0
60.90	2529.0
61.90	2501.0
62.90	1877.0
63.90	190.0
66.80	178.0
67.90	5405.0
68.90	5446.0
69.90	416.0
71.80	297.0
72.90	2384.0
73.90	9110.0
74.90	26552.0
75.90	2304.0
76.90	261.0
77.80	193.0
78.80	1986.0
79.80	549.0
80.80	1958.0
81.80	446.0
86.90	2024.0
87.80	1834.0
90.70	262.0
91.90	1481.0
92.90	2311.0
93.90	6189.0
94.90	50736.0
95.90	3357.0
96.90	103.0
103.80	236.0
105.80	260.0
115.80	218.0
116.70	331.0
117.80	195.0
118.80	301.0
127.70	239.0
129.80	188.0
134.70	116.0
136.70	112.0
140.80	545.0
142.80	584.0
147.70	122.0
154.70	119.0
172.90	285.0
173.80	38184.0
174.80	2707.0
175.80	36808.0
176.80	2337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB109