

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
 Data File : VU062965.D
 Acq On : 23 Jan 2025 12:37
 Operator : MD/SY
 Sample : VSTD0.1
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 24 00:11:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 24 00:10:41 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	8959	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	10224	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3666	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	431	0.072	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.709	65	777	0.114	ug/L	0.02
7) 1,2-Dichloropropane-d6	6.687	67	581	0.098	ug/L	0.00
8) Toluene-d8	7.887	98	1531	0.101	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.745	84	368	0.073	ug/L	0.00
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.597	62	601	0.078	ug/L #	1
6) Trichloroethene	6.544	95	823	0.129	ug/L	97
9) 1,2-Dibromoethane	8.924	107	350	0.091	ug/L #	93
12) 1,2,3-Trichloropropane	10.814	75	298	0.076	ug/L	96
13) 1,2-Dibromo-3-chloropr...	13.008	75	103	0.135	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
Data File : VU062965.D
Acq On : 23 Jan 2025 12:37
Operator : MD/SY
Sample : VSTD0.1
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 24 00:11:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 24 00:10:41 2025
Response via : Initial Calibration




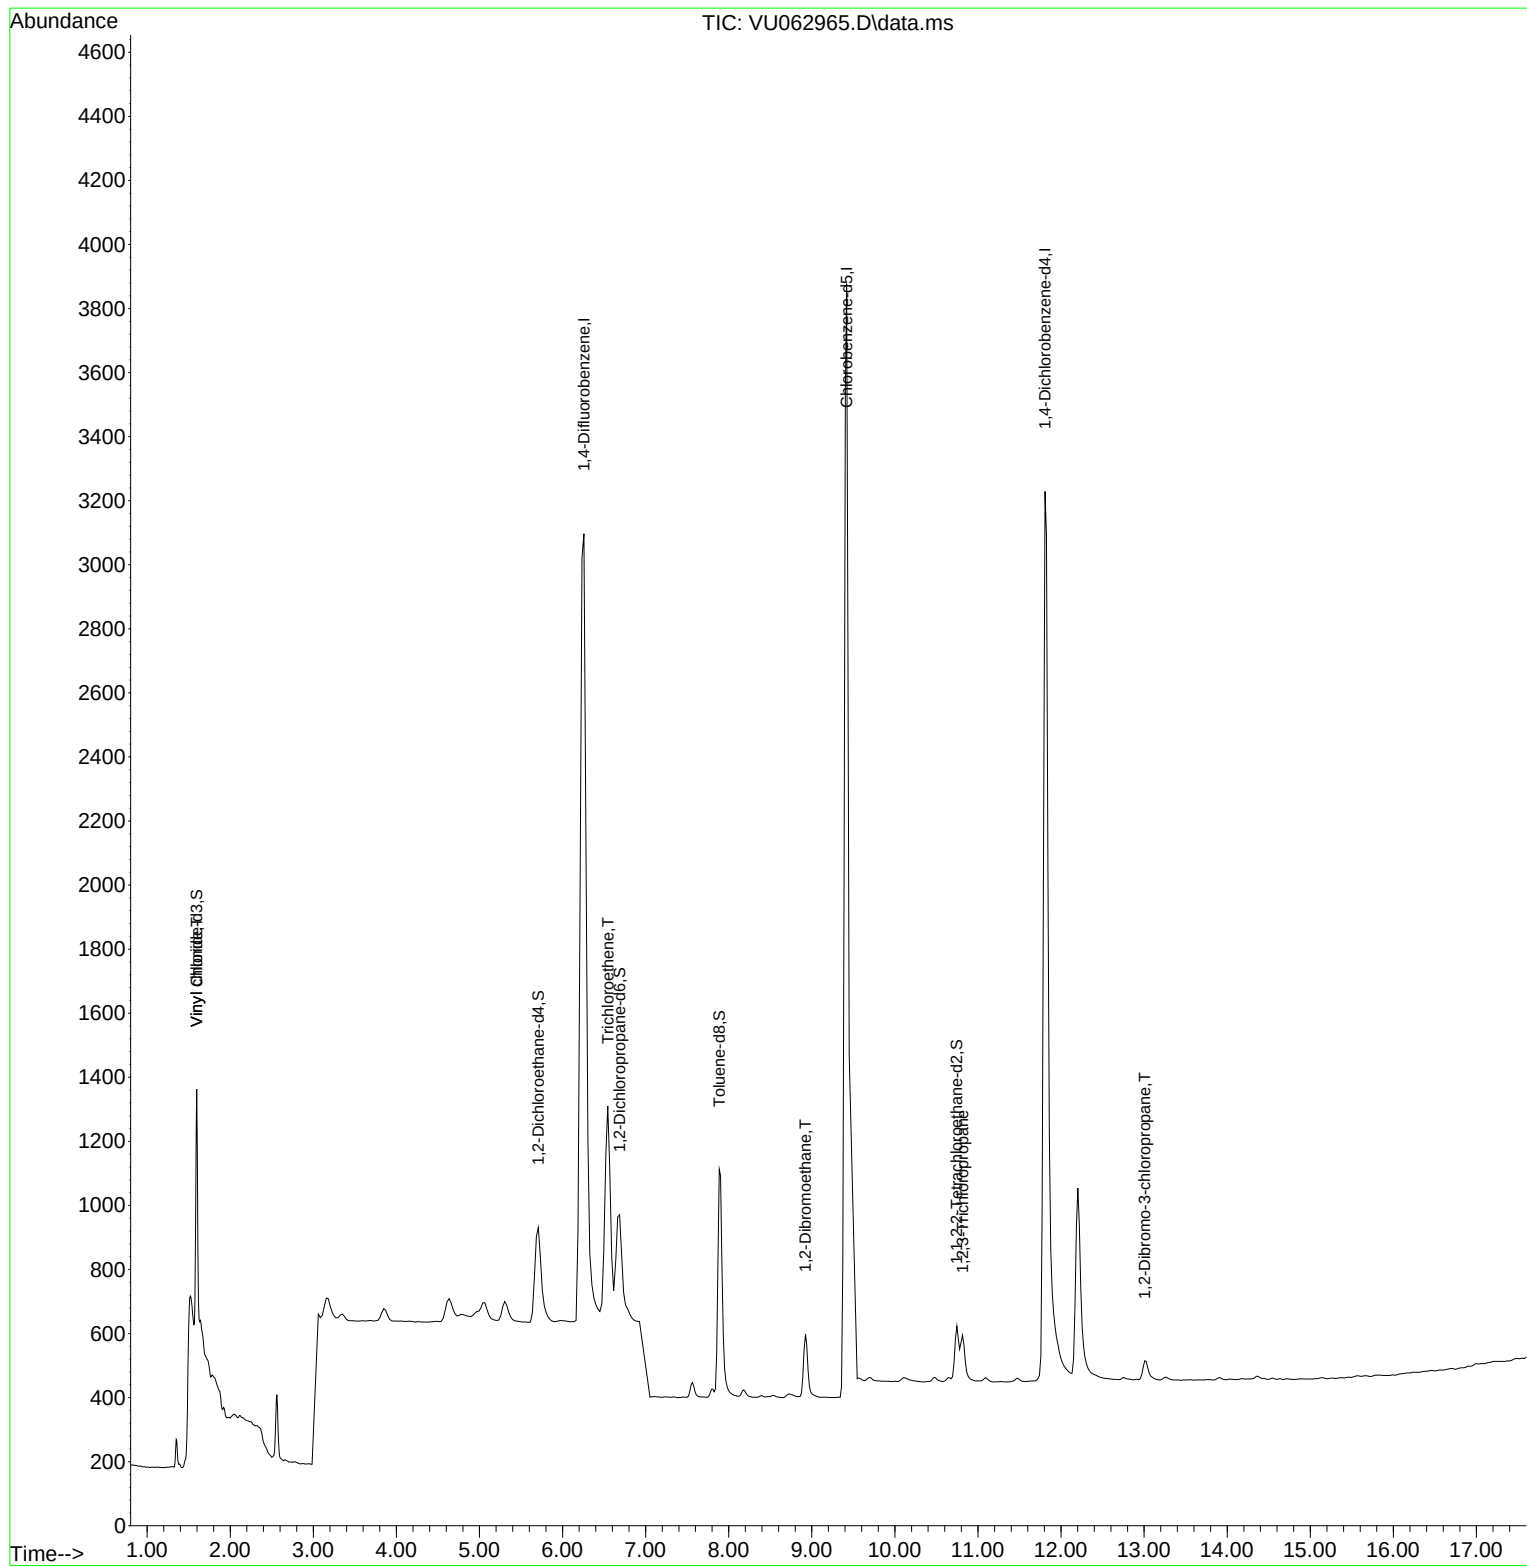


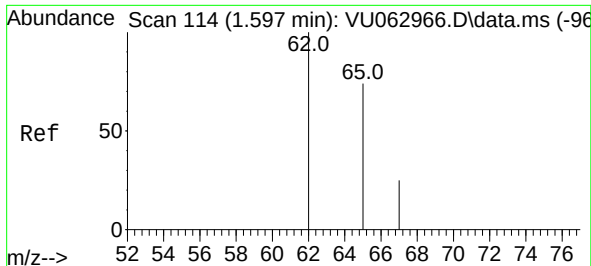

#3
Vinyl chloride
Concen: 0.078 ug/L
RT: 1.597 min Scan# 114
Delta R.T. -0.000 min
Lab File: VU062965.D
Acq: 23 Jan 2025 12:37




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 62 Resp: 601
Ion Ratio Lower Upper
62 100
64 147.4 43.2 80.2#

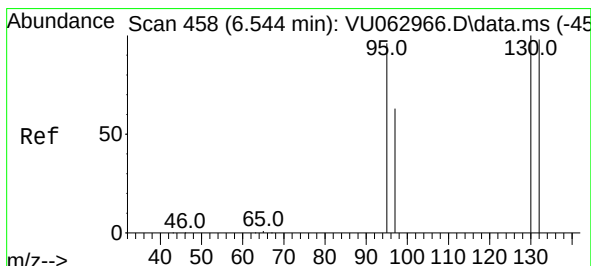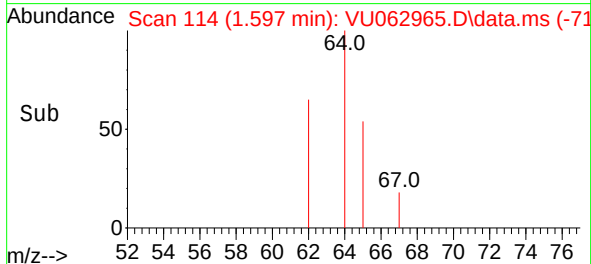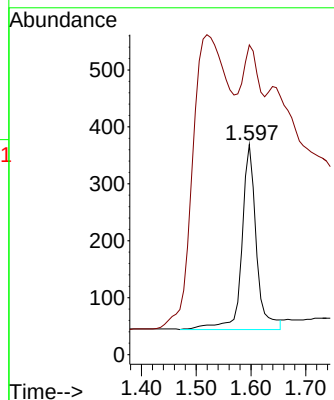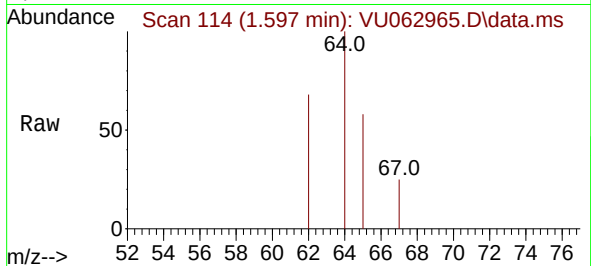

#6
Trichloroethene
Concen: 0.129 ug/L
RT: 6.544 min Scan# 458
Delta R.T. -0.000 min
Lab File: VU062965.D
Acq: 23 Jan 2025 12:37


Tgt Ion: 95 Resp: 823
Ion Ratio Lower Upper
95 100
97 73.5 47.0 87.4
132 101.8 71.5 132.9
130 102.3 72.7 135.1

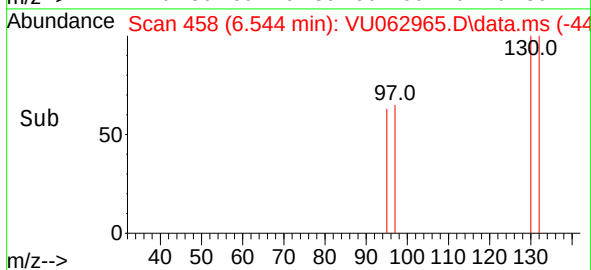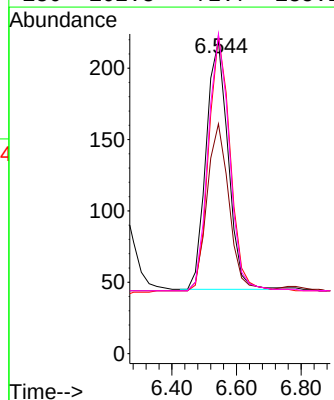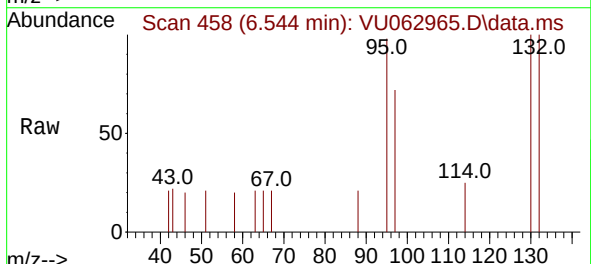



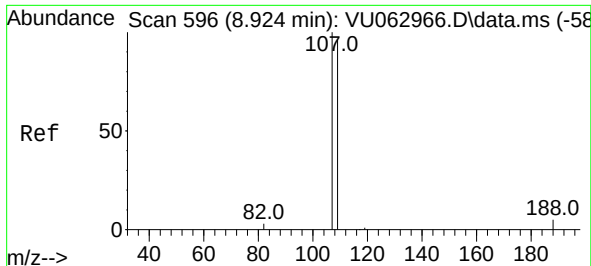


#9
1,2-Dibromoethane
Concen: 0.091 ug/L
RT: 8.924 min Scan# 596
Delta R.T. -0.000 min
Lab File: VU062965.D
Acq: 23 Jan 2025 12:37


Instrument :
MSVOA_U
ClientSampleId :

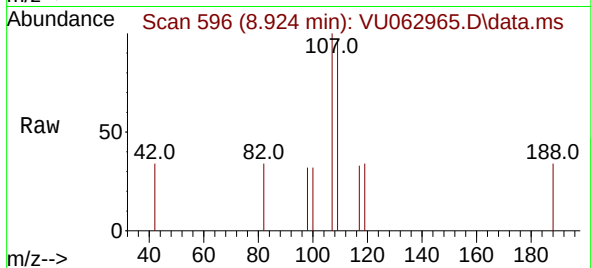



Tgt Ion:107 Resp: 350
Ion Ratio Lower Upper
107 100
109 97.1 67.1 124.7
188 34.1 9.6 14.4#

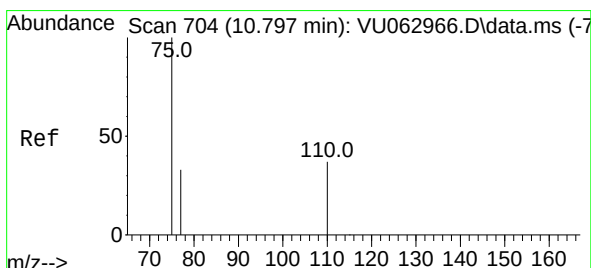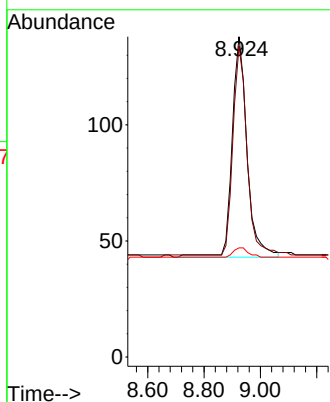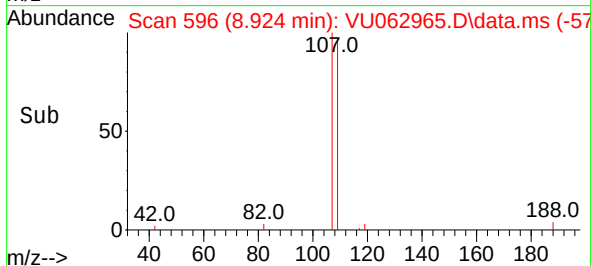


#12
1,2,3-Trichloropropane
Concen: 0.076 ug/L
RT: 10.814 min Scan# 705
Delta R.T. 0.017 min
Lab File: VU062965.D
Acq: 23 Jan 2025 12:37

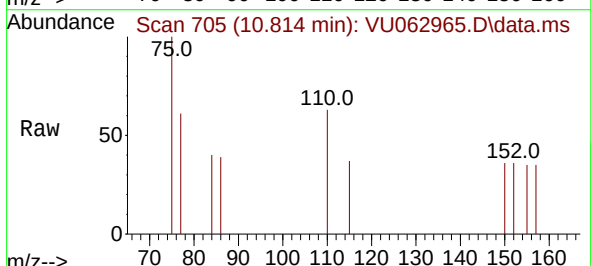


Tgt Ion: 75 Resp: 298
Ion Ratio Lower Upper
75 100
110 41.6 34.3 51.5
77 36.9 27.0 40.6

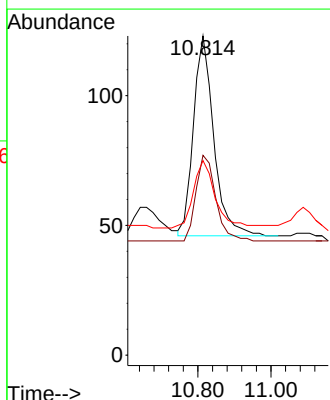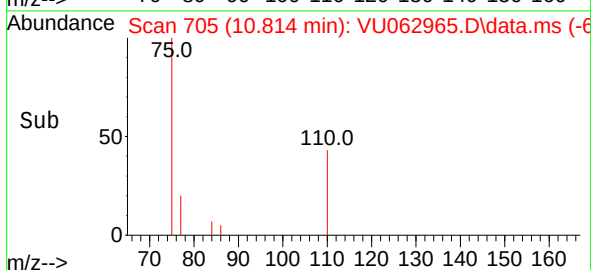

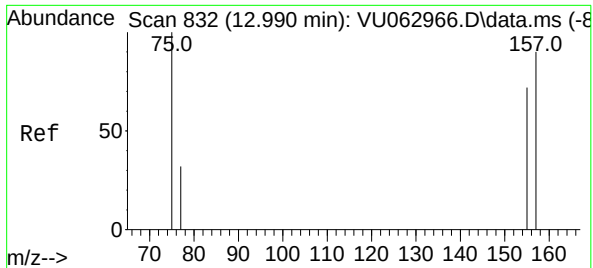

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.135 ug/L
 RT: 13.008 min Scan# 84
 Delta R.T. 0.017 min
 Lab File: VU062965.D
 Acq: 23 Jan 2025 12:37

Instrument :
 MSVOA_U
 ClientSampleId :

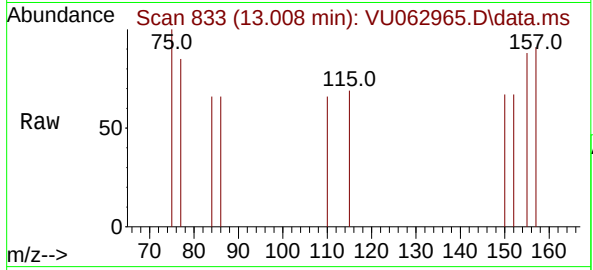

Tgt Ion: 75	Resp:	103
Ion Ratio	Lower	Upper
75	100	
157	91.0	73.2 109.8
155	88.1	63.3 94.9

