

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
 Data File : VU062970.D
 Acq On : 23 Jan 2025 16:50
 Operator : MD/SY
 Sample : VU0123WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 24 02:21:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 24 00:16:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	9031	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	11500	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152	3805	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2137	0.444	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3674	0.465	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2606	0.420	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.887	98	7756	0.453	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2385	0.467	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	94.000%		
Target Compounds						
6) Trichloroethene	6.544	95	163	0.018	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
Data File : VU062970.D
Acq On : 23 Jan 2025 16:50
Operator : MD/SY
Sample : VU0123WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 24 02:21:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 24 00:16:16 2025
Response via : Initial Calibration

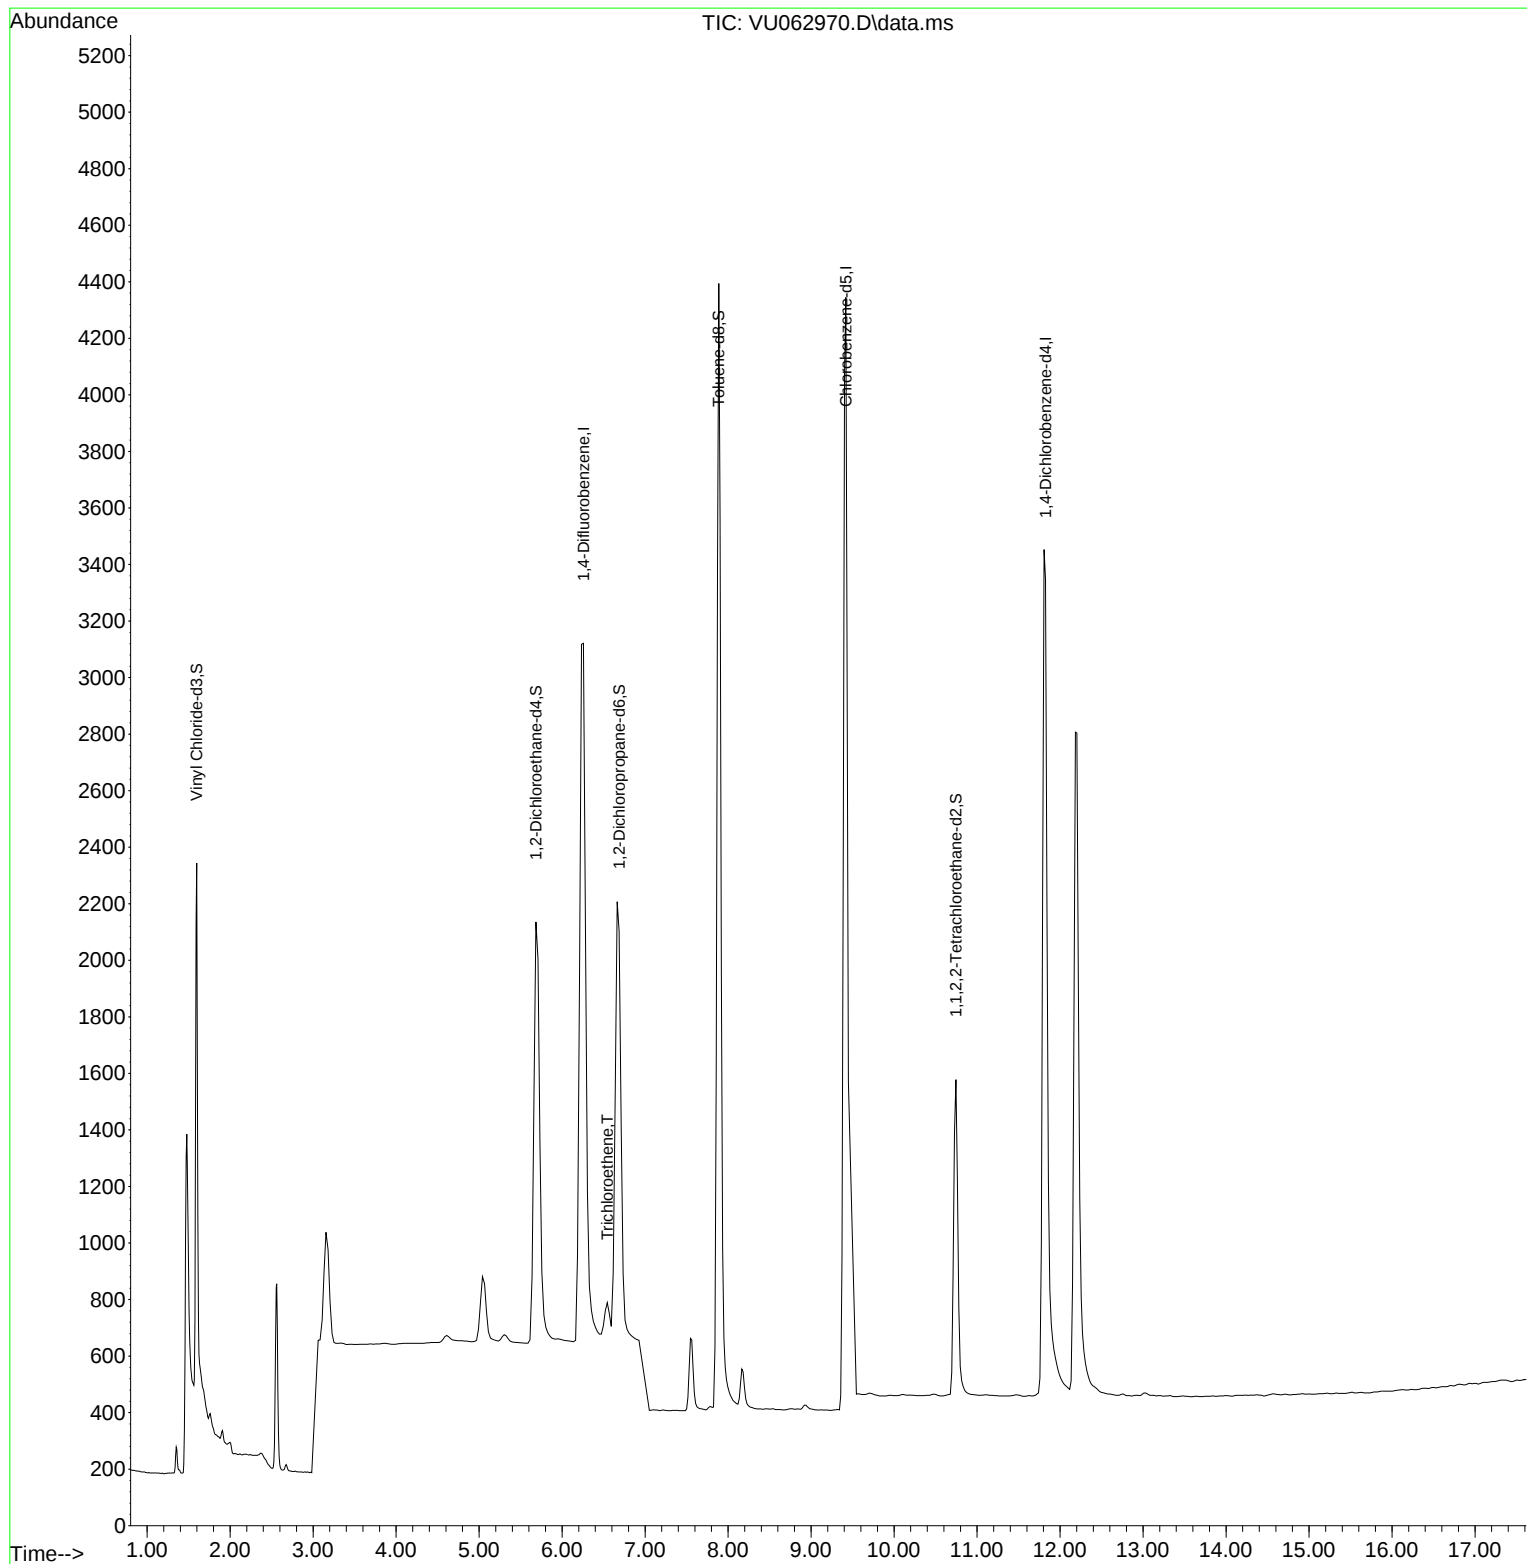

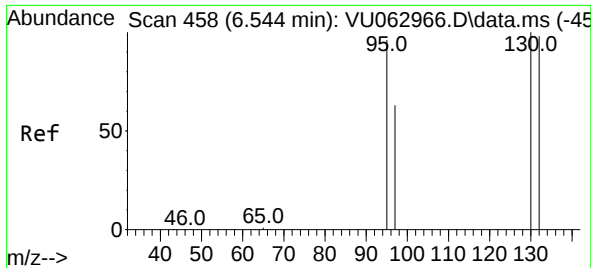

#6
 Trichloroethene
 Concen: 0.018 ug/L
 RT: 6.544 min Scan# 4
 Delta R.T. -0.000 min
 Lab File: VU062970.D
 Acq: 23 Jan 2025 16:50

Instrument :
 MSVOA_U
 ClientSampleId :

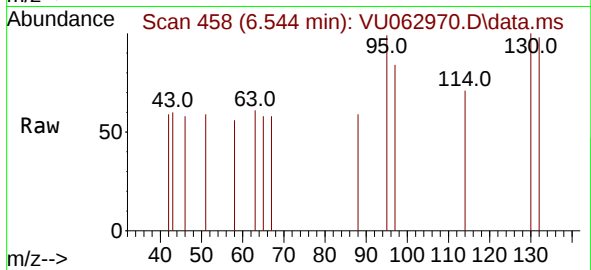

Tgt Ion: 95	Resp: 163
Ion Ratio	Lower Upper
95	100
97	84.8 47.0 87.4
132	98.7 71.5 132.9
130	101.3 72.7 135.1

